

Sample Name : [Glu1]-Fibrinopeptide B  
 Cat No: RP20439  
 Lot No : E8549221E  
 Time Processed : 17:46:43  
 Month-Day-Year Processed : 05/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

| Time  | Module     | Command       | Value |
|-------|------------|---------------|-------|
| 0.01  | Pumps      | Pump A B.Conc | 5     |
| 25.00 | Pumps      | Pump A B.Conc | 65    |
| 25.01 | Pumps      | Pump A B.Conc | 95    |
| 31.00 | Pumps      | Pump A B.Conc | 95    |
| 31.01 | Pumps      | Pump A B.Conc | 5     |
| 35.00 | Pumps      | Pump A B.Conc | 5     |
| 40.00 | Controller | Stop          |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

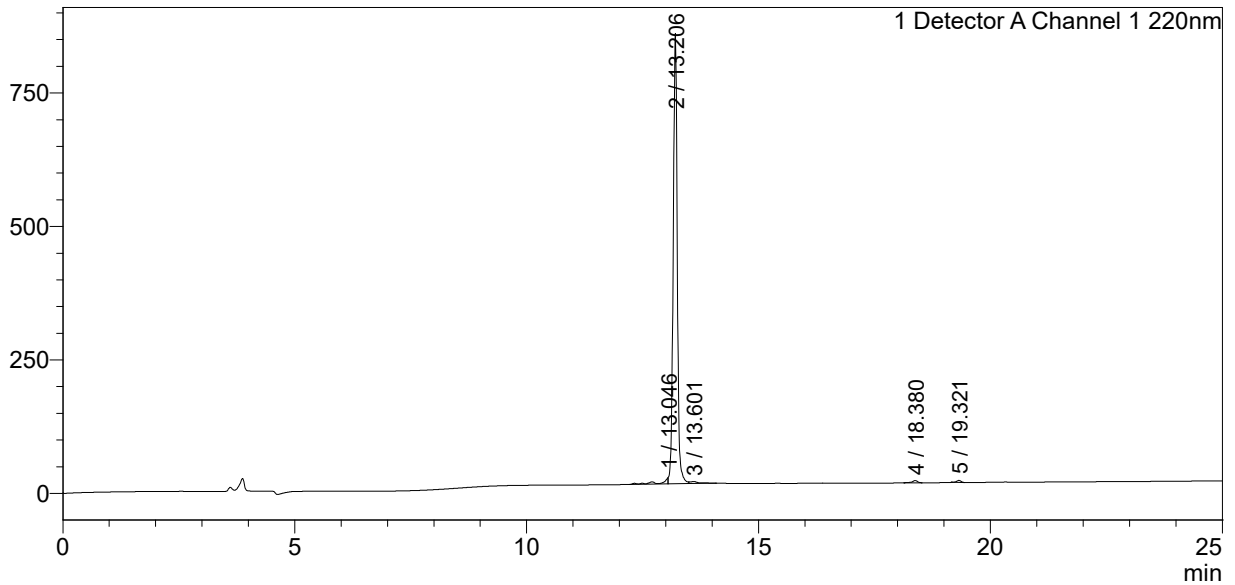

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height | Area%   |
|-------|-----------|---------|--------|---------|
| 1     | 13.046    | 119598  | 11036  | 2.220   |
| 2     | 13.206    | 5157735 | 843839 | 95.735  |
| 3     | 13.601    | 53037   | 3890   | 0.984   |
| 4     | 18.380    | 32650   | 4253   | 0.606   |
| 5     | 19.321    | 24497   | 3757   | 0.455   |
| Total |           | 5387516 | 866775 | 100.000 |