


Mass Spectrum

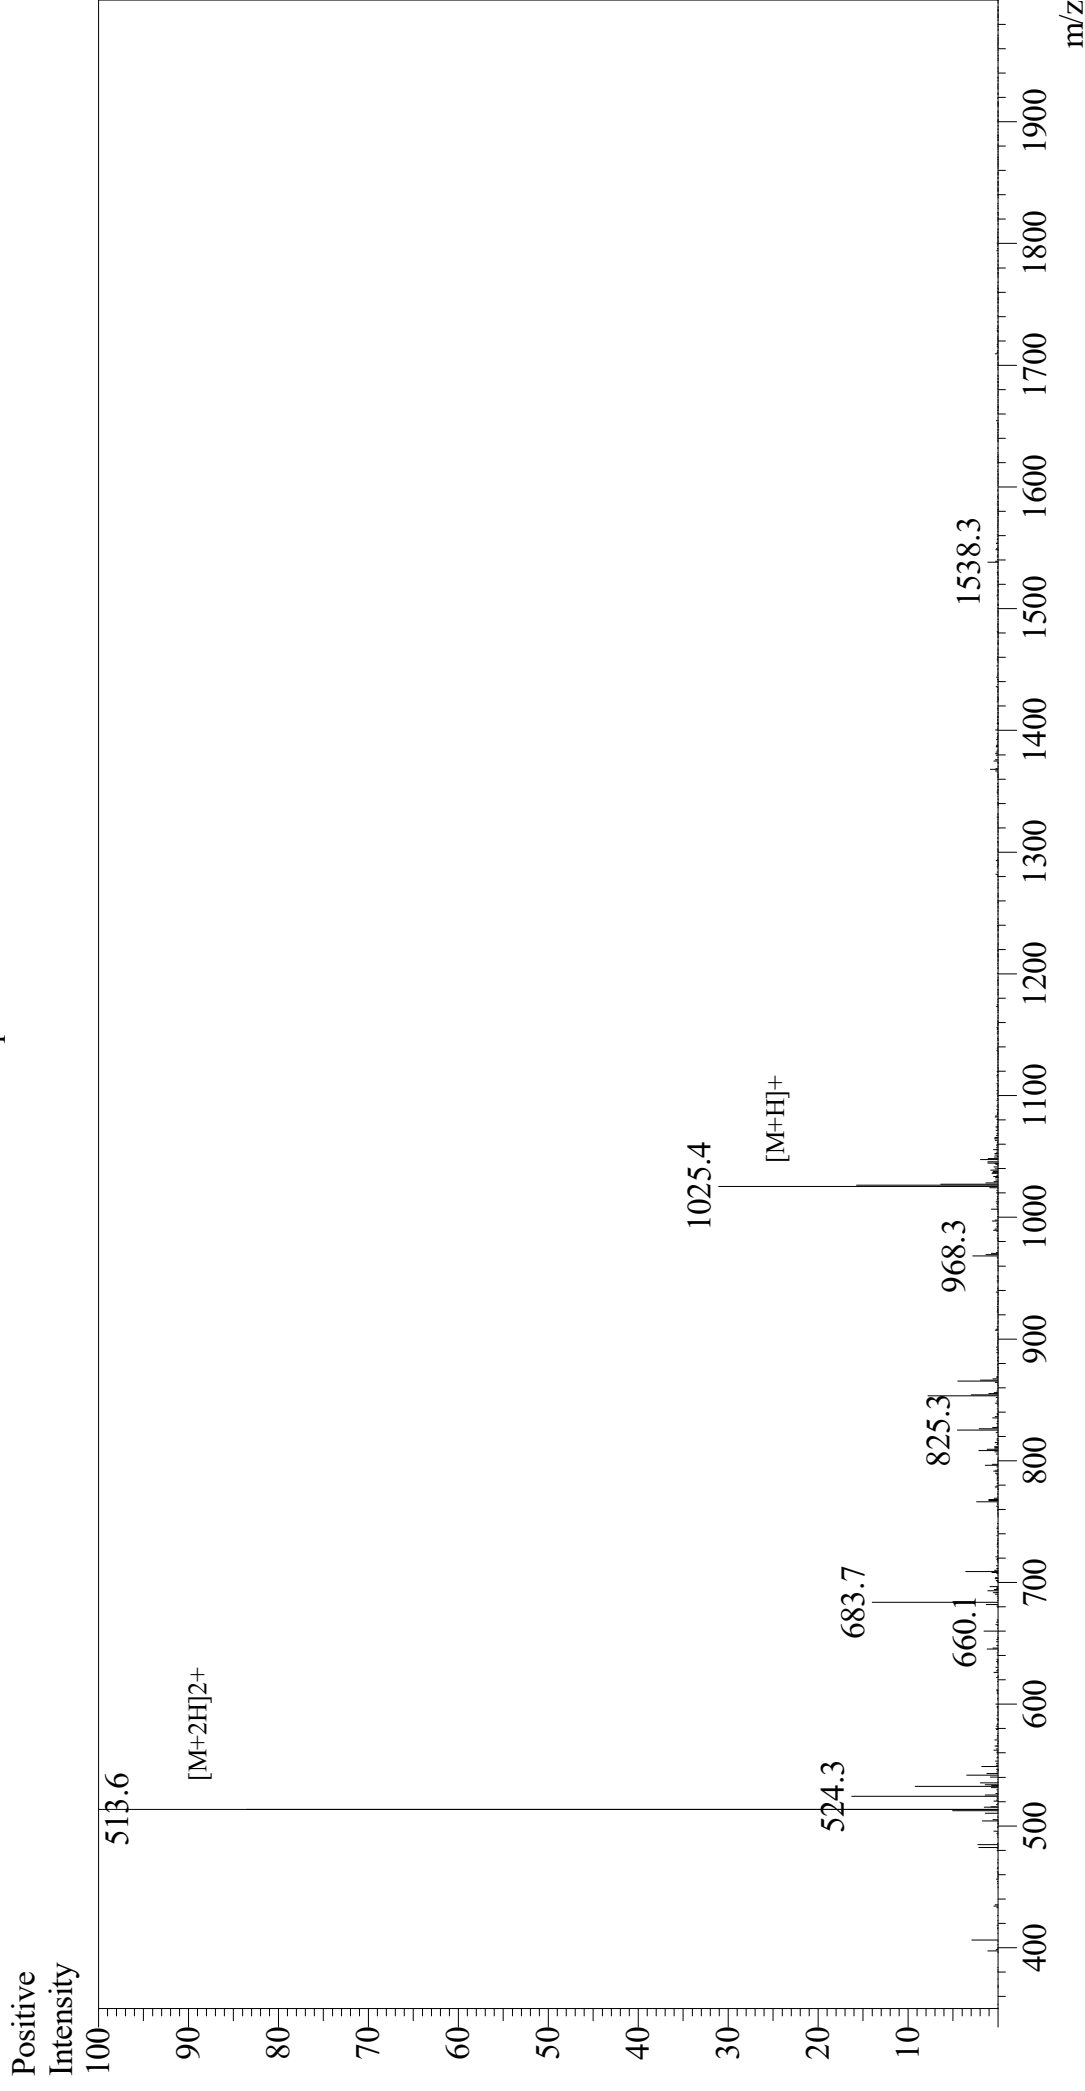

Sample Information

Month-Day Processed : 11/25/21
 Time Processed : 19:22:10
 Injection Volume : 0.2
 Sample Name : RGD
 Cat No. : RP20297
 Lot No. : E7857921K
 Theoretical MW : 1025.06
 Observed MW : 1025.2

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH