

Sample Name :p53(17-26)  
 Cat No. :RP20338  
 Lot No. :E4942119I  
 Time Processed :7:42:25  
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

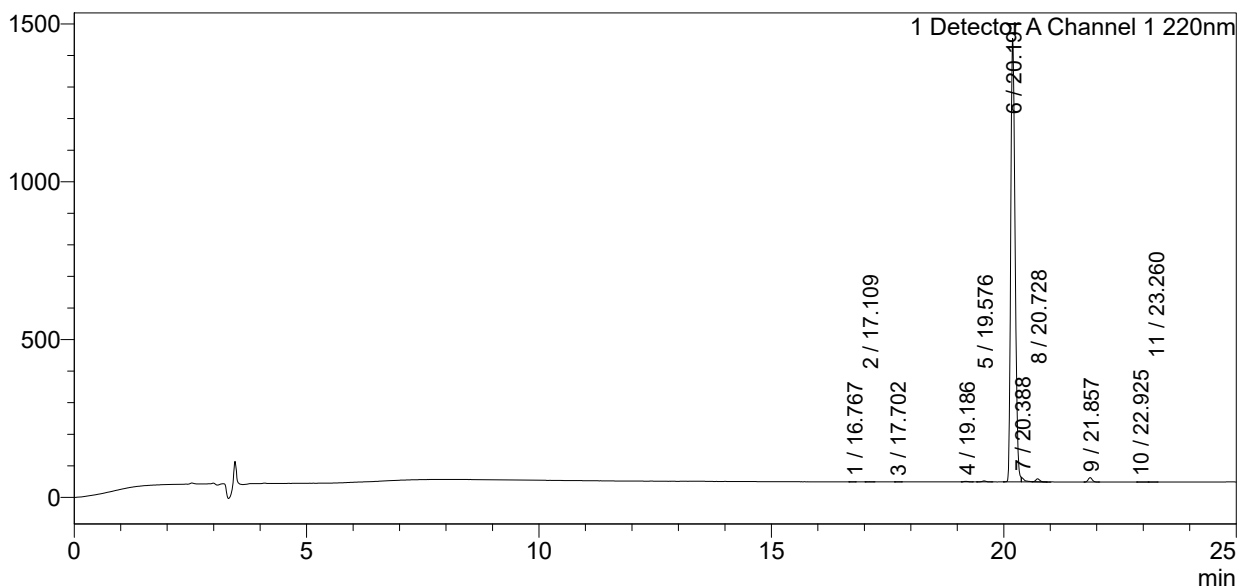

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.767	1124	218	0.012
2	17.109	2125	410	0.023
3	17.702	1716	338	0.018
4	19.186	11229	1909	0.120
5	19.576	18732	3114	0.199
6	20.191	9141611	1404600	97.351
7	20.388	70497	13993	0.751
8	20.728	56714	9589	0.604
9	21.857	83441	13965	0.889
10	22.925	1619	237	0.017
11	23.260	1570	206	0.017
Total		9390376	1448580	100.000