

Sample Name : Angiotensin I, human
 Cat. No. : RP11251
 Lot. No. : PE5481902
 Time Processed : 10:28:07
 Month-Day-Year Processed : 02/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

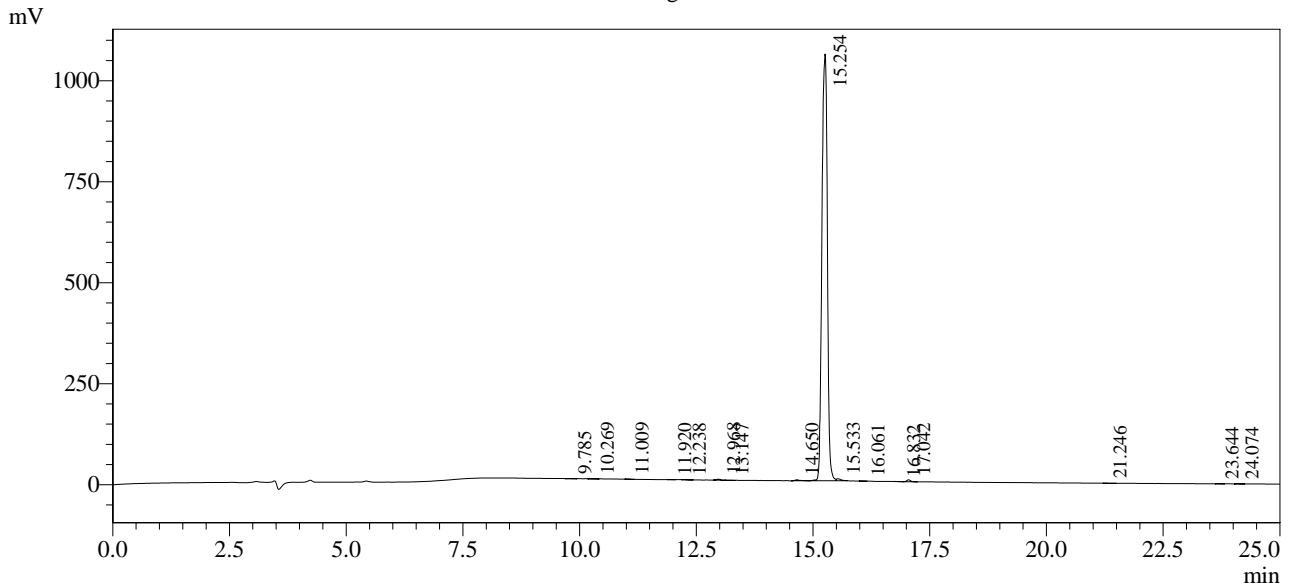

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.785	1551	254	0.018
2	10.269	1531	202	0.018
3	11.009	1189	147	0.014
4	11.920	1020	204	0.012
5	12.238	2209	515	0.025
6	12.968	14719	2747	0.170
7	13.147	1210	137	0.014
8	14.650	16616	2453	0.192
9	15.254	8566096	1056304	98.851
10	15.533	28568	4737	0.330
11	16.061	1072	256	0.012
12	16.832	1248	236	0.014
13	17.042	25295	4785	0.292
14	21.246	1219	102	0.014
15	23.644	1028	197	0.012
16	24.074	1079	144	0.012
Total		8665648	1073422	100.000