


Mass Spectrum

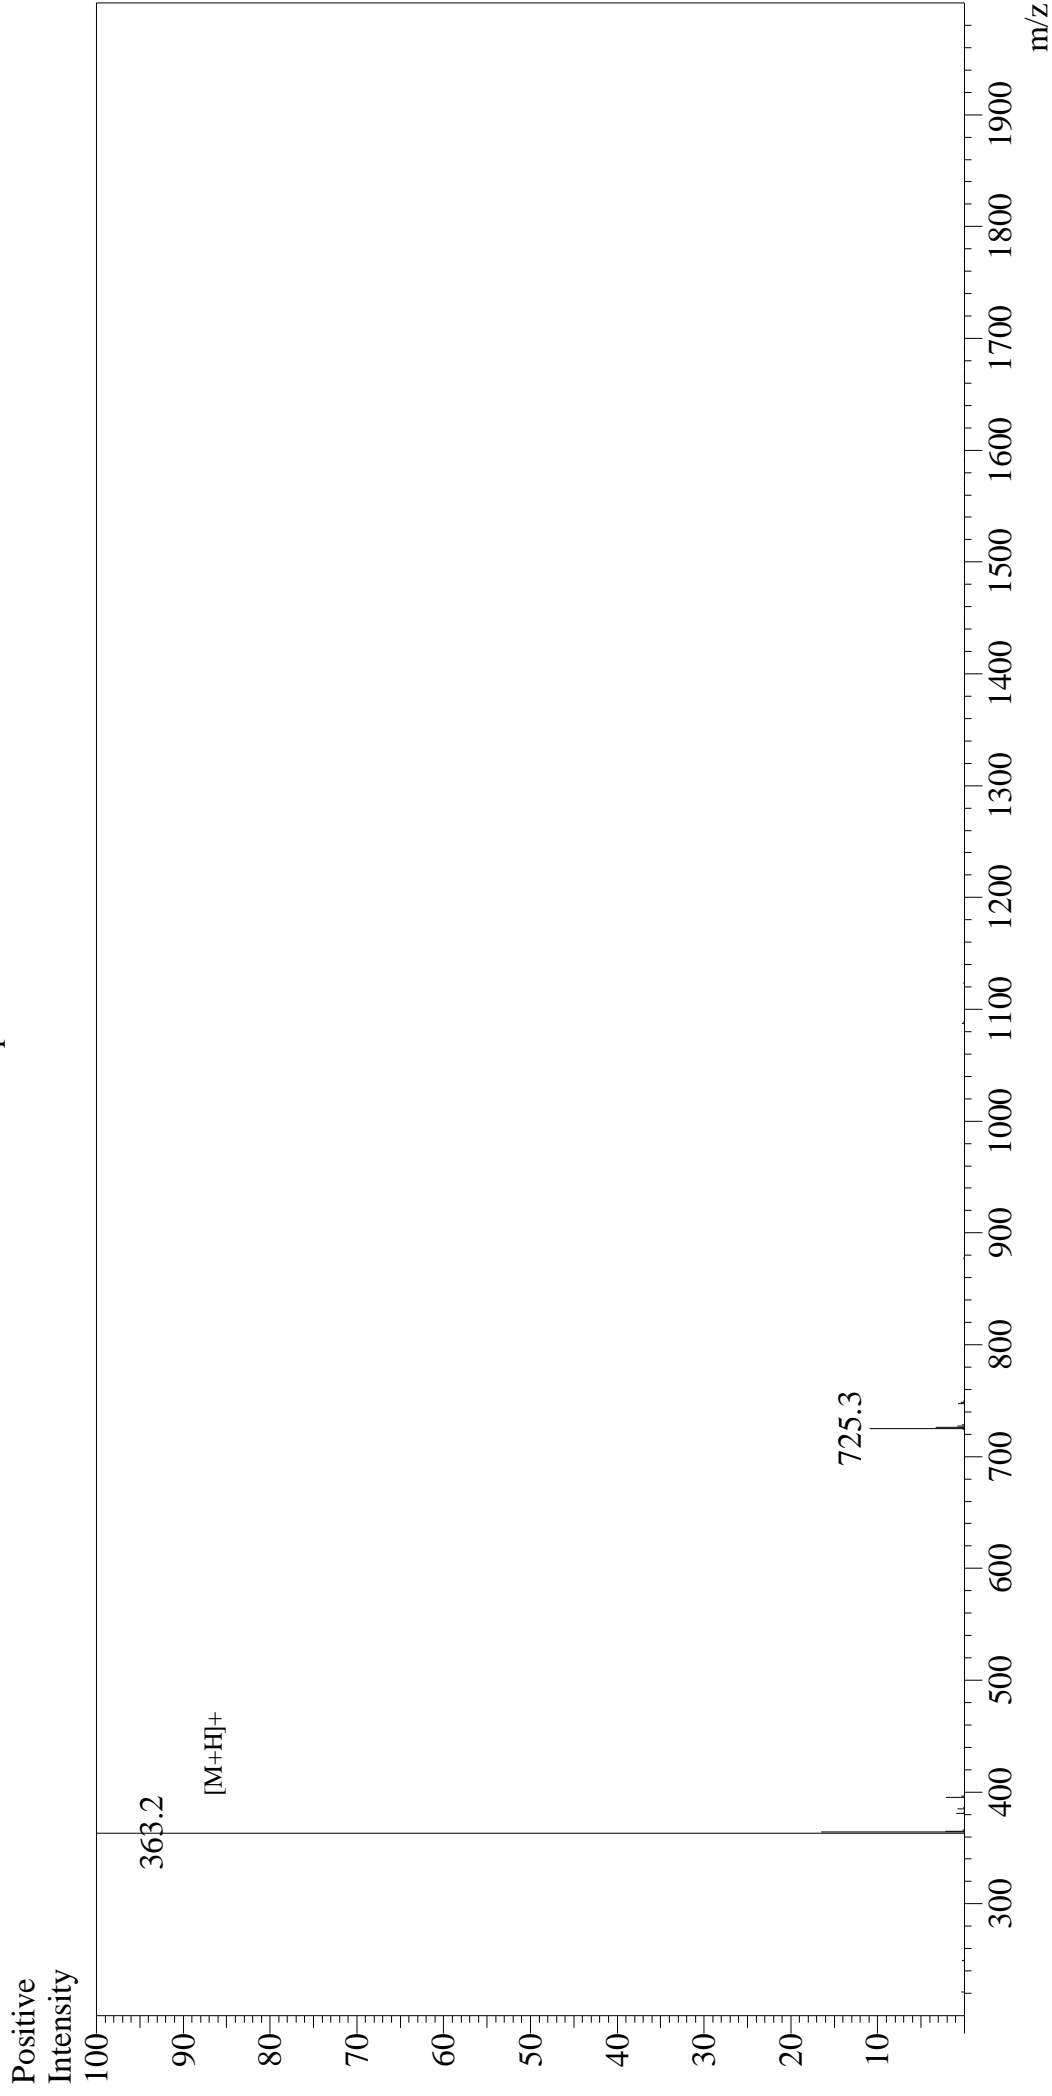

Sample Information

User : Gary
Month-Day Processed : 11/09/18
Time Processed : 20:22:13
Injection Volume : 0.2
Sample Name : Thyrotropin-Releasing Hormone (TRH)
Cat No. : RPI0112
Lot No. : PE5651810
Theoretical MW : 362.38
Observed MW : 362.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH