

Sample Information

Sample Name : PAR-4 Agonist Peptide, amide
 Cat. No. : RP11529
 Lot. No. : PE9611801

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

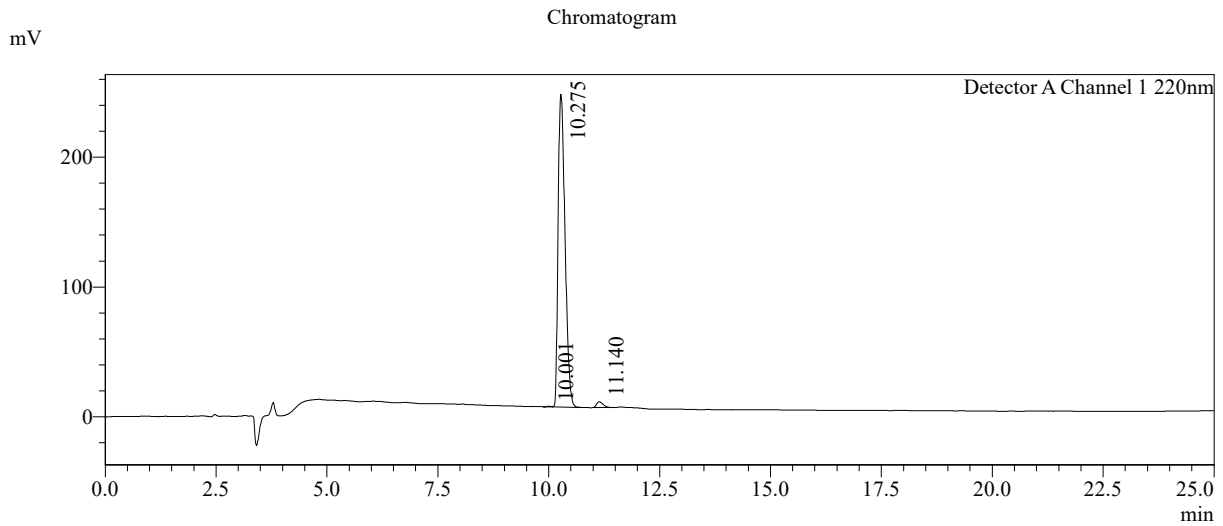

Peak Table

Detector A Channel 1 220nm						
Peak#	Ret. Time	Height	Area	Height%	Area%	
1	10.001	504	2851	0.205	0.107	
2	10.275	240918	2617269	97.983	98.194	
3	11.140	4456	45274	1.812	1.699	
Total		245878	2665394	100.000	100.000	