

Sample Name:IKKy NBD Inhibitory Peptide  
 Cat No: RP20478  
 Lot No: E2007221D  
 Time Processed :9:15:54 PM  
 Month-Day-Year Processed :05/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

### <Chromatogram>

mV

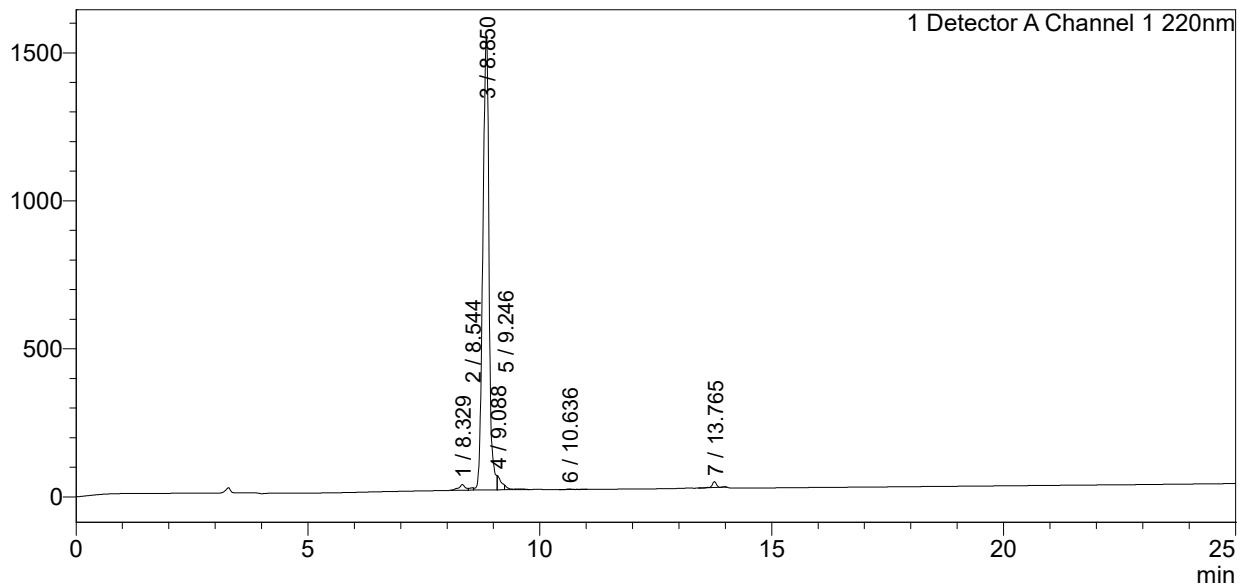

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.329	187189	18874	1.252
2	8.544	45389	7729	0.304
3	8.850	14231021	1535074	95.159
4	9.088	271603	48402	1.816
5	9.246	90331	15767	0.604
6	10.636	12608	2090	0.084
7	13.765	116872	19755	0.781
Total		14955013	1647692	100.000