

Sample Name : CNP (1-22), human
 Cat. No. :RP11110
 Lot. No. :PE9041811
 Time Processed : 10:19:06
 Month-Day-Year Processed : 01/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

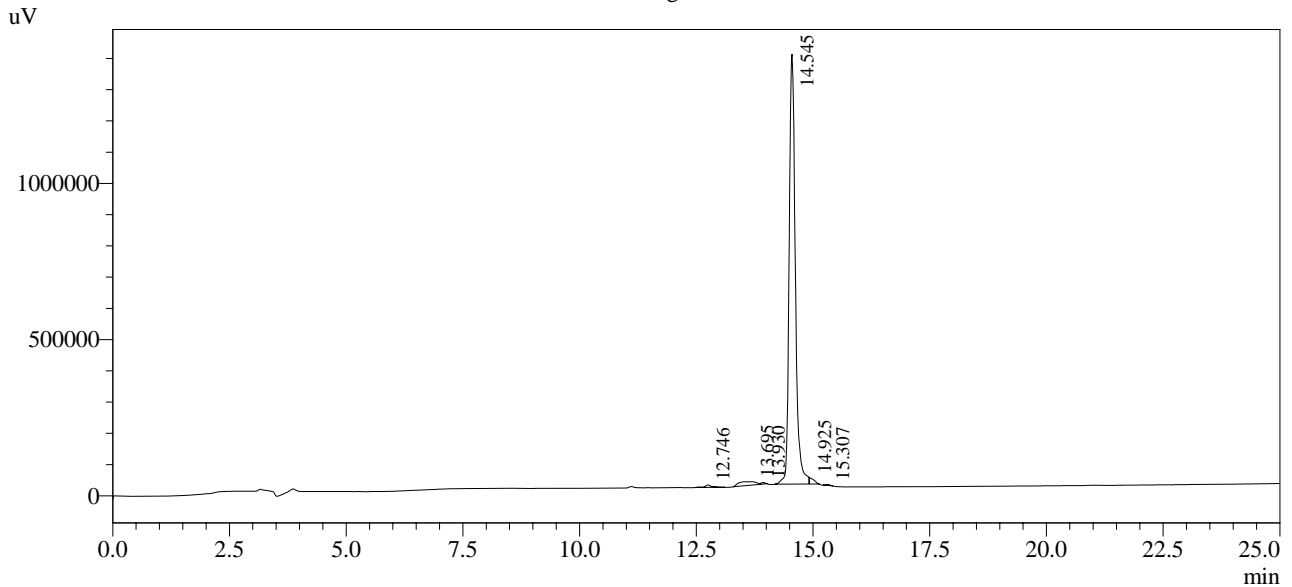

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.746	82374	7707	0.620
2	13.695	310270	10538	2.337
3	13.930	27180	4572	0.205
4	14.545	12698409	1376095	95.640
5	14.925	137073	20949	1.032
6	15.307	21935	3503	0.165
Total		13277242	1423365	100.000