

Sample Name :Autocamtide 2
 Cat No.: RP10271
 Lot No.: E8009020I
 Time Processed :8:20:58 AM
 Month-Day-Year Processed :09/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

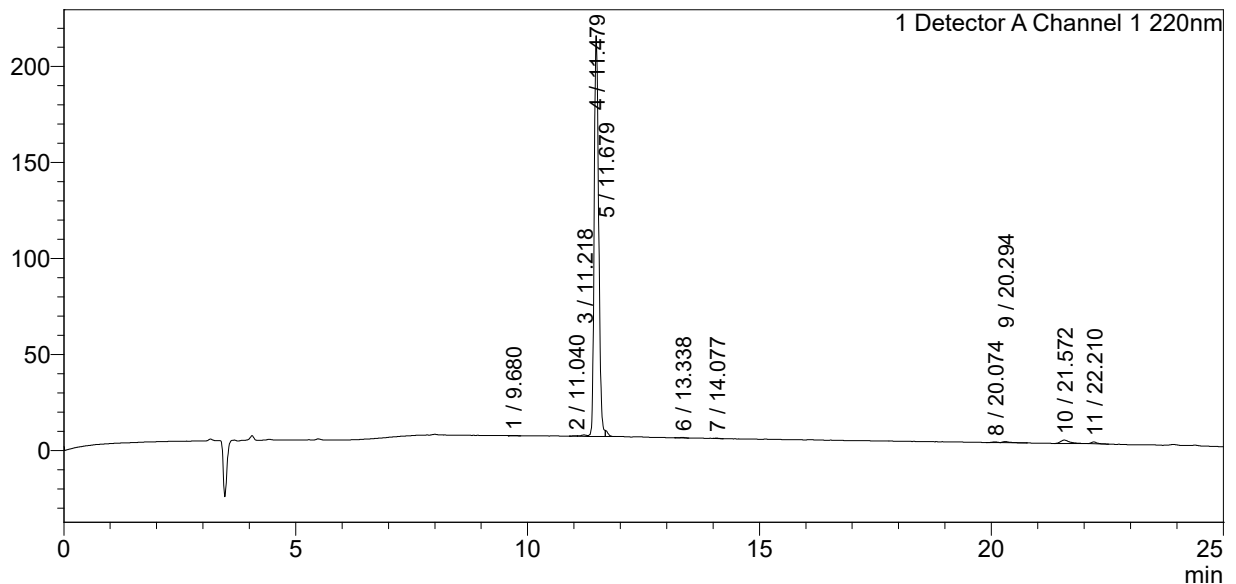

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.680	1265	156	0.085
2	11.040	1503	206	0.101
3	11.218	6348	696	0.428
4	11.479	1414845	208765	95.431
5	11.679	11868	3172	0.801
6	13.338	1855	284	0.125
7	14.077	1178	222	0.079
8	20.074	3450	390	0.233
9	20.294	7651	680	0.516
10	21.572	24598	1792	1.659
11	22.210	8030	937	0.542
Total		1482592	217300	100.000