


Mass Spectrum

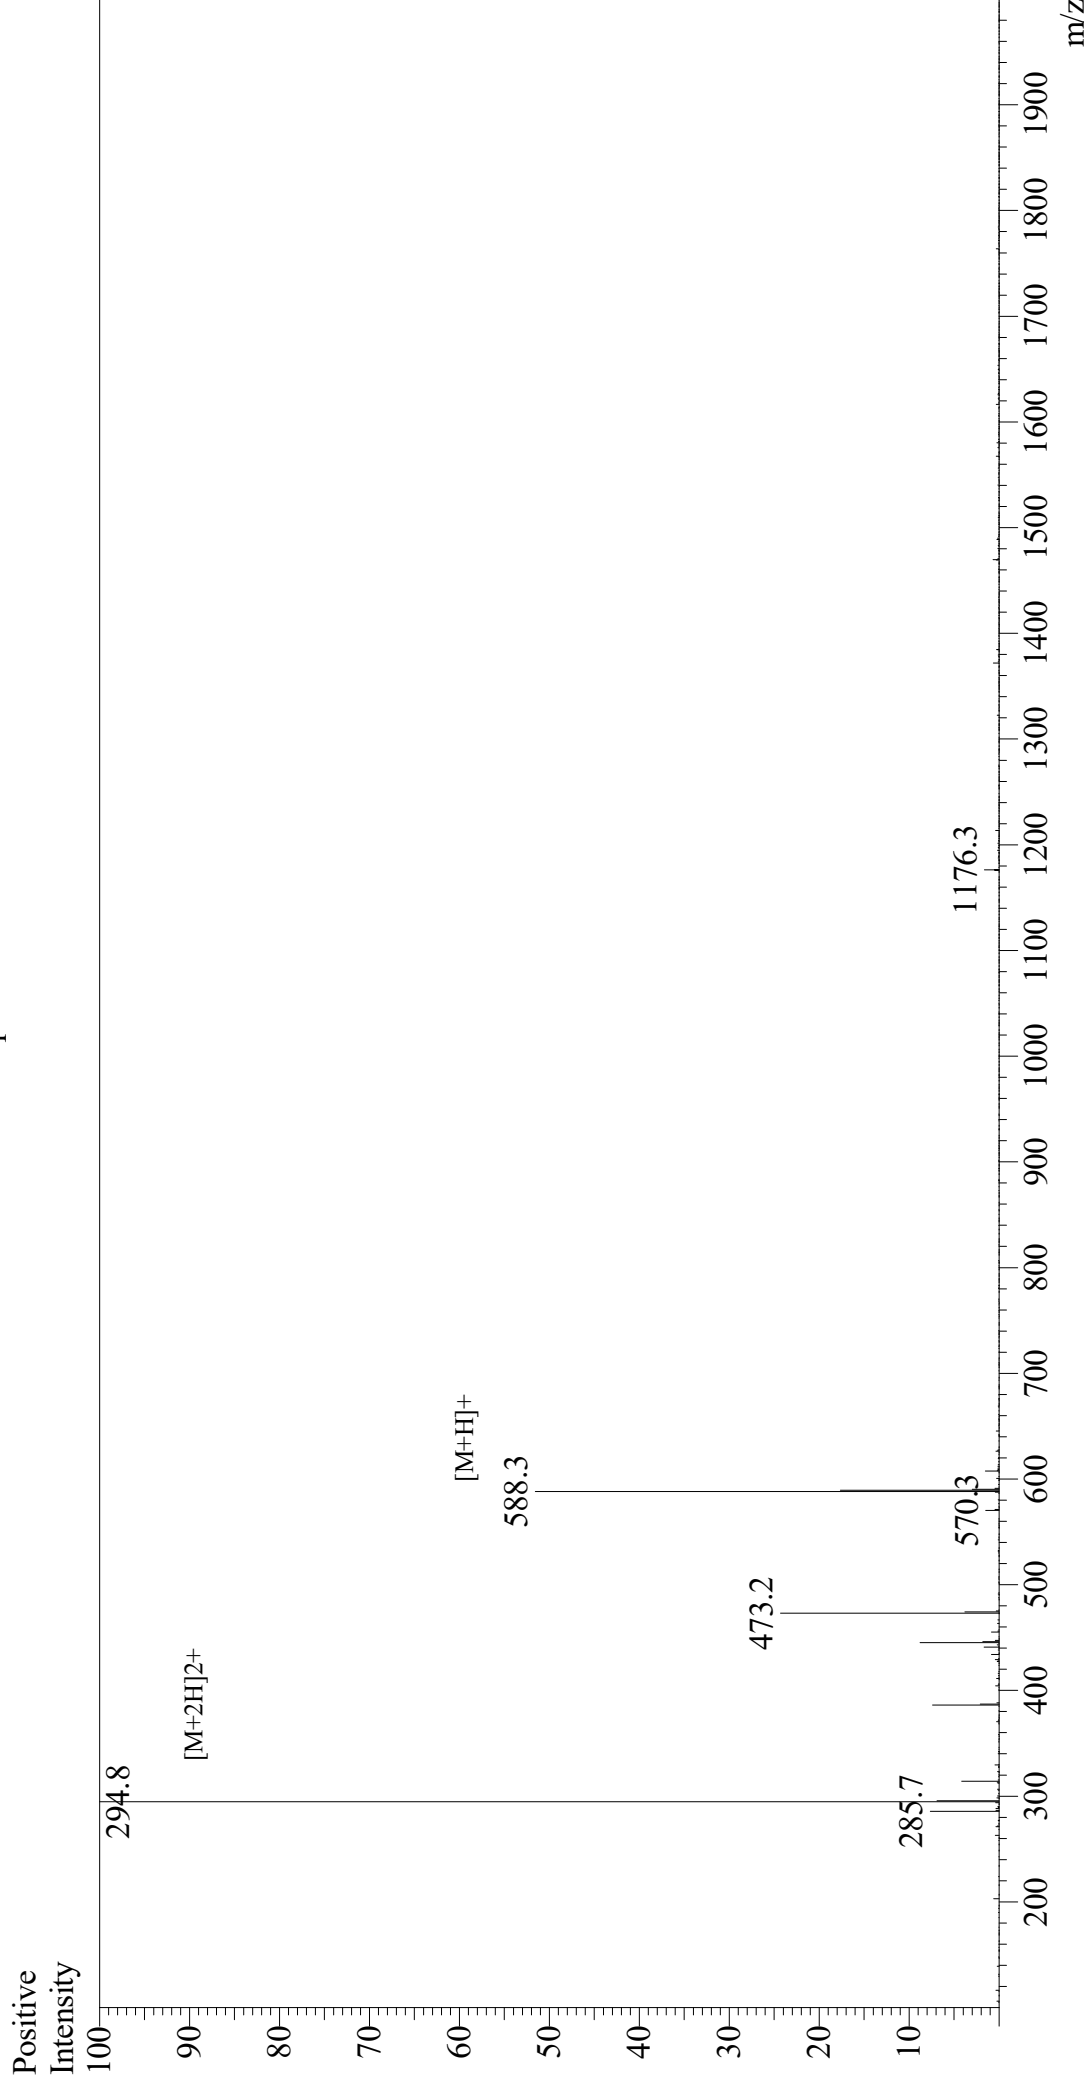

Sample Information

Acquired by : Gary
 Month-Day Processed : 06/10/19
 Time Processed : 07:37:16 PM
 Injection Volume : 0.3
 Sample Name : GRGDSP
 Cat. No. : RP20255
 Lot. No. : E4192519F
 Theoretical MW : 587.59
 Observed MW : 587.6

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200
 Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH