

Sample Name : U4248BL070-1
 Cat. No. : RP20423
 Lot. No. : PE4681612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

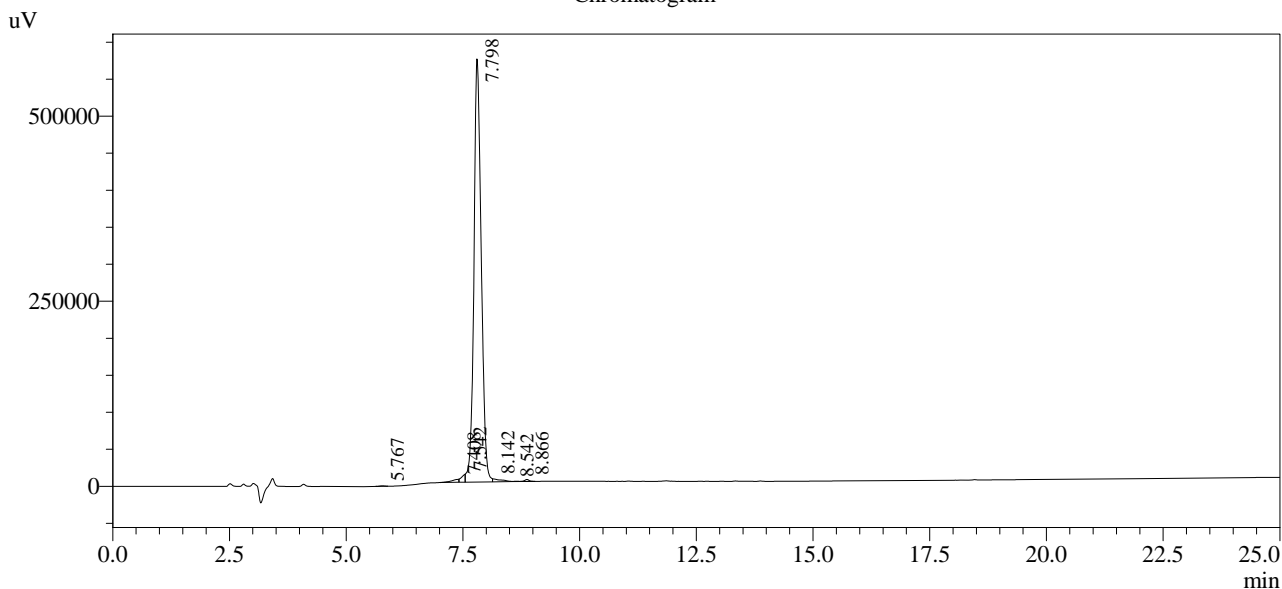

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.767	4446	659	0.069
2	7.408	44069	4145	0.688
3	7.542	61552	10658	0.960
4	7.798	6225290	571767	97.141
5	8.142	51983	4070	0.811
6	8.542	5679	398	0.089
7	8.866	15520	2591	0.242
Total		6408539	594288	100.000