

Sample Name :Influenza A NP(366-374) Strain A/PR/8/35
 Cat No. :RP20267
 Lot No. :E0909919G
 Time Processed :7:00:49
 Month-Day-Year Processed :07/02/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

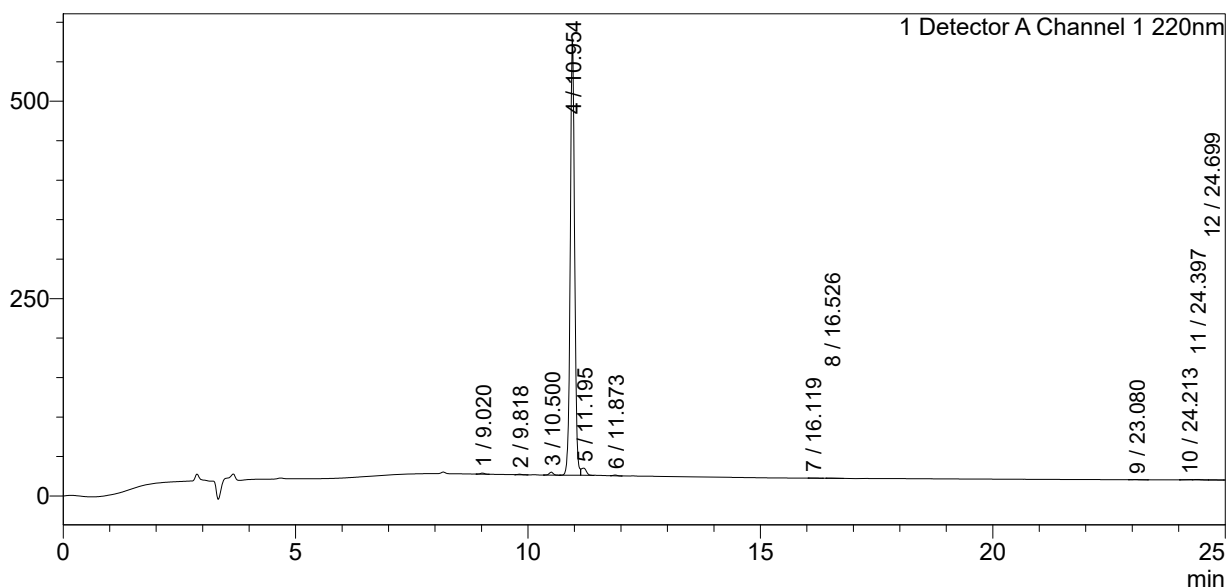

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.020	8106	1360	0.217
2	9.818	3959	704	0.106
3	10.500	22139	3706	0.592
4	10.954	3613308	551921	96.617
5	11.195	67073	9038	1.793
6	11.873	5792	1015	0.155
7	16.119	1378	181	0.037
8	16.526	1788	184	0.048
9	23.080	2623	249	0.070
10	24.213	5500	583	0.147
11	24.397	7086	618	0.189
12	24.699	1092	123	0.029
Total		3739845	569681	100.000