

Sample Name : A-779  
 Cat. No. : RP11249  
 Lot. No. : PE5331610

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

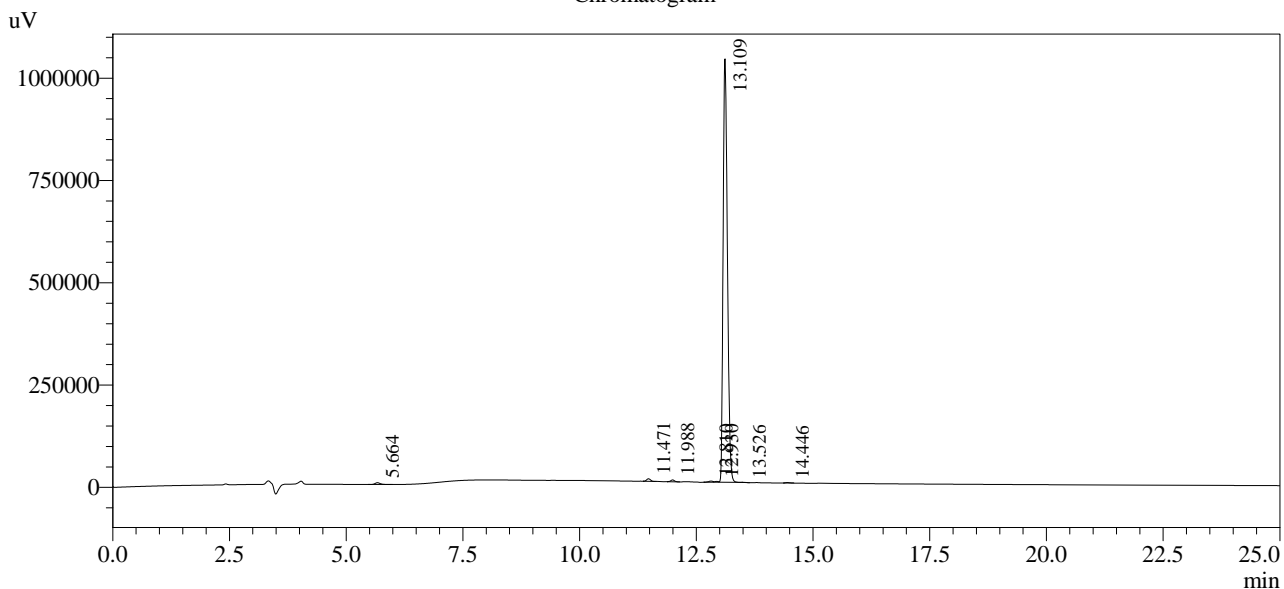

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.664	31887	4336	0.471
2	11.471	35106	6233	0.519
3	11.988	25607	4648	0.378
4	12.810	17540	2941	0.259
5	12.930	11985	2224	0.177
6	13.109	6635850	1033391	98.070
7	13.526	1797	413	0.027
8	14.446	6673	1069	0.099
Total		6766445	1055256	100.000