

Sample Name :Abz-FR-K (Dnp)-P-OH
 Cat No. :RP20115
 Lot No. :E6298420J
 Time Processed :10:32:50 AM
 Month-Day-Year Processed :10/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

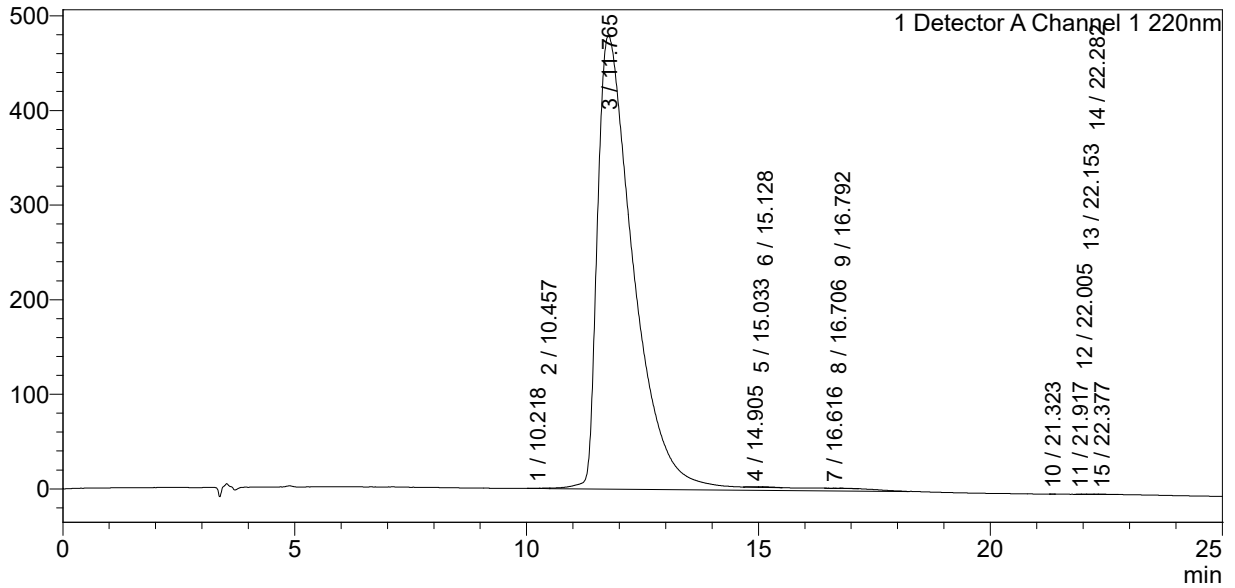

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.218	2871	270	0.011
2	10.457	5427	536	0.021
3	11.765	26319455	479328	99.808
4	14.905	7287	559	0.028
5	15.033	3310	621	0.013
6	15.128	9658	685	0.037
7	16.616	2677	269	0.010
8	16.706	1621	304	0.006
9	16.792	5283	399	0.020
10	21.323	1201	237	0.005
11	21.917	1085	205	0.004
12	22.005	1463	229	0.006
13	22.153	2309	285	0.009
14	22.282	1518	308	0.006

Peak#	Ret. Time	Area	Height	Area%
15	22.377	4940	337	0.019
Total		26370105	484572	100.000