

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human  
 Cat. No. :RP11110  
 Lot. No. :E2474720J  
 Time Processed : 2:52:53 PM  
 Month-Day-Year Processed : 10/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

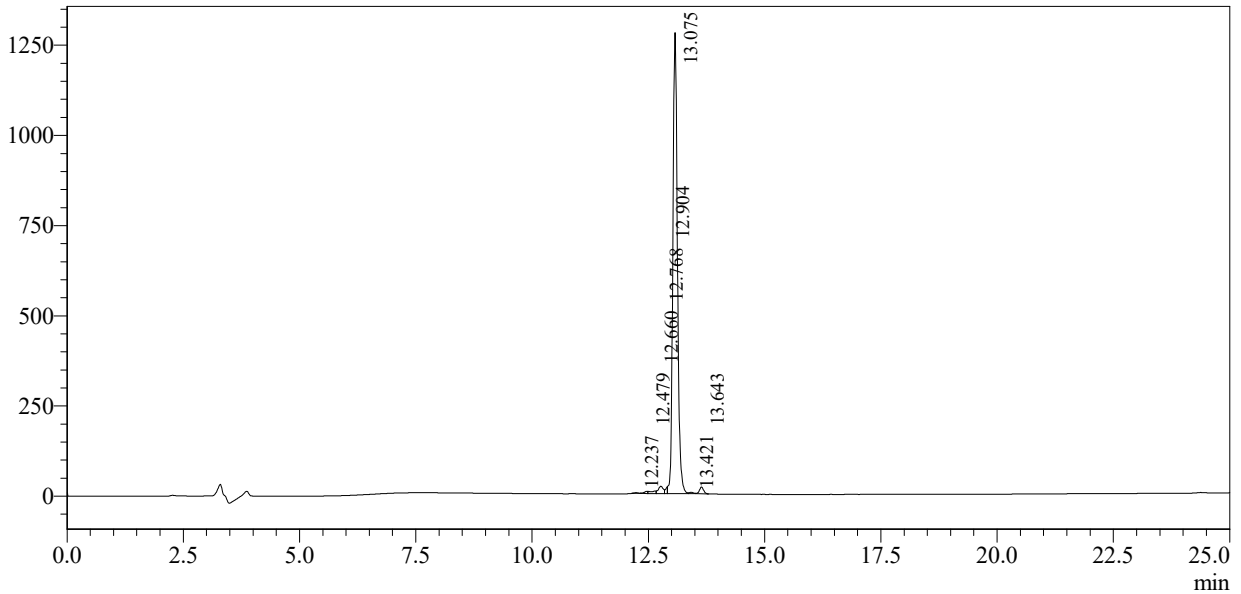

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.237	12744	2013	0.138
2	12.479	33269	6188	0.360
3	12.660	60602	7210	0.655
4	12.768	152395	20375	1.648
5	12.904	51327	18021	0.555
6	13.075	8797918	1277901	95.134
7	13.421	25490	3819	0.276
8	13.643	114200	18768	1.235
Total		9247945	1354294	100.000