

Sample Name : Human Papillomavirus (HPV) E7 protein (49 - 57)
 Cat. No. : RP20249
 Lot. No. : PE1781610


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

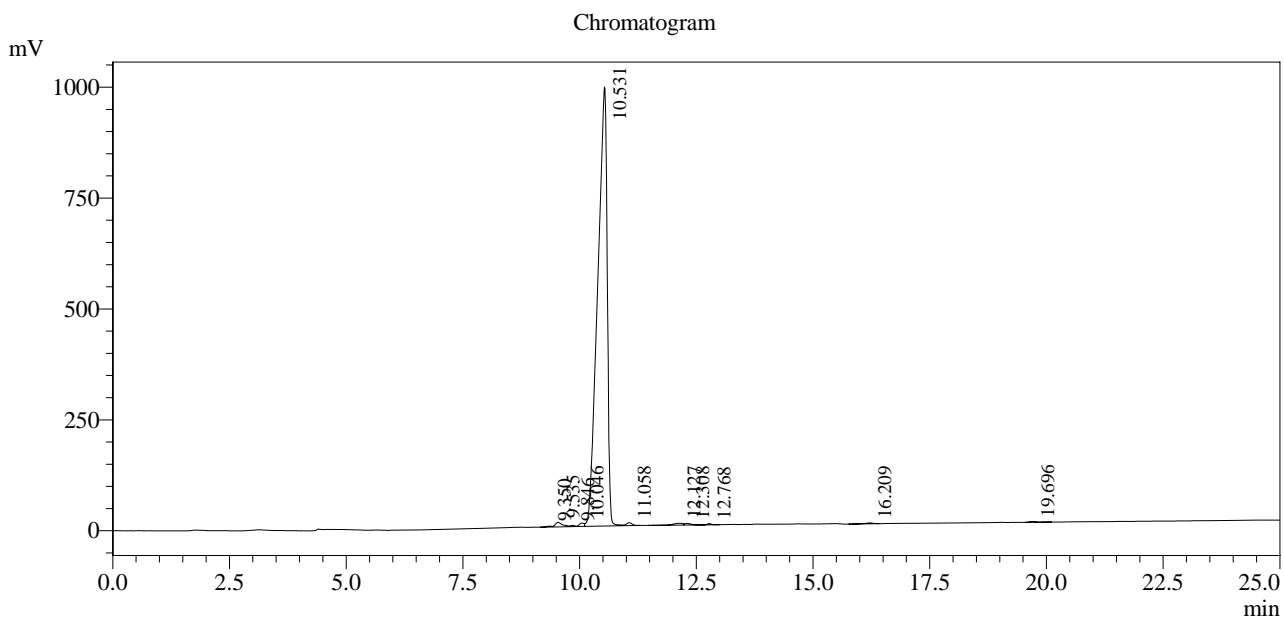

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.350	13466	1941	0.093
2	9.535	109069	10141	0.756
3	9.846	17968	2542	0.125
4	10.046	55032	7590	0.381
5	10.531	14012649	990216	97.116
6	11.058	59344	6505	0.411
7	12.127	67167	4398	0.466
8	12.308	36604	3576	0.254
9	12.768	19562	2703	0.136
10	16.209	24477	1898	0.170
11	19.696	13382	1458	0.093
Total		14428719	1032969	100.000