Mass Spectrum

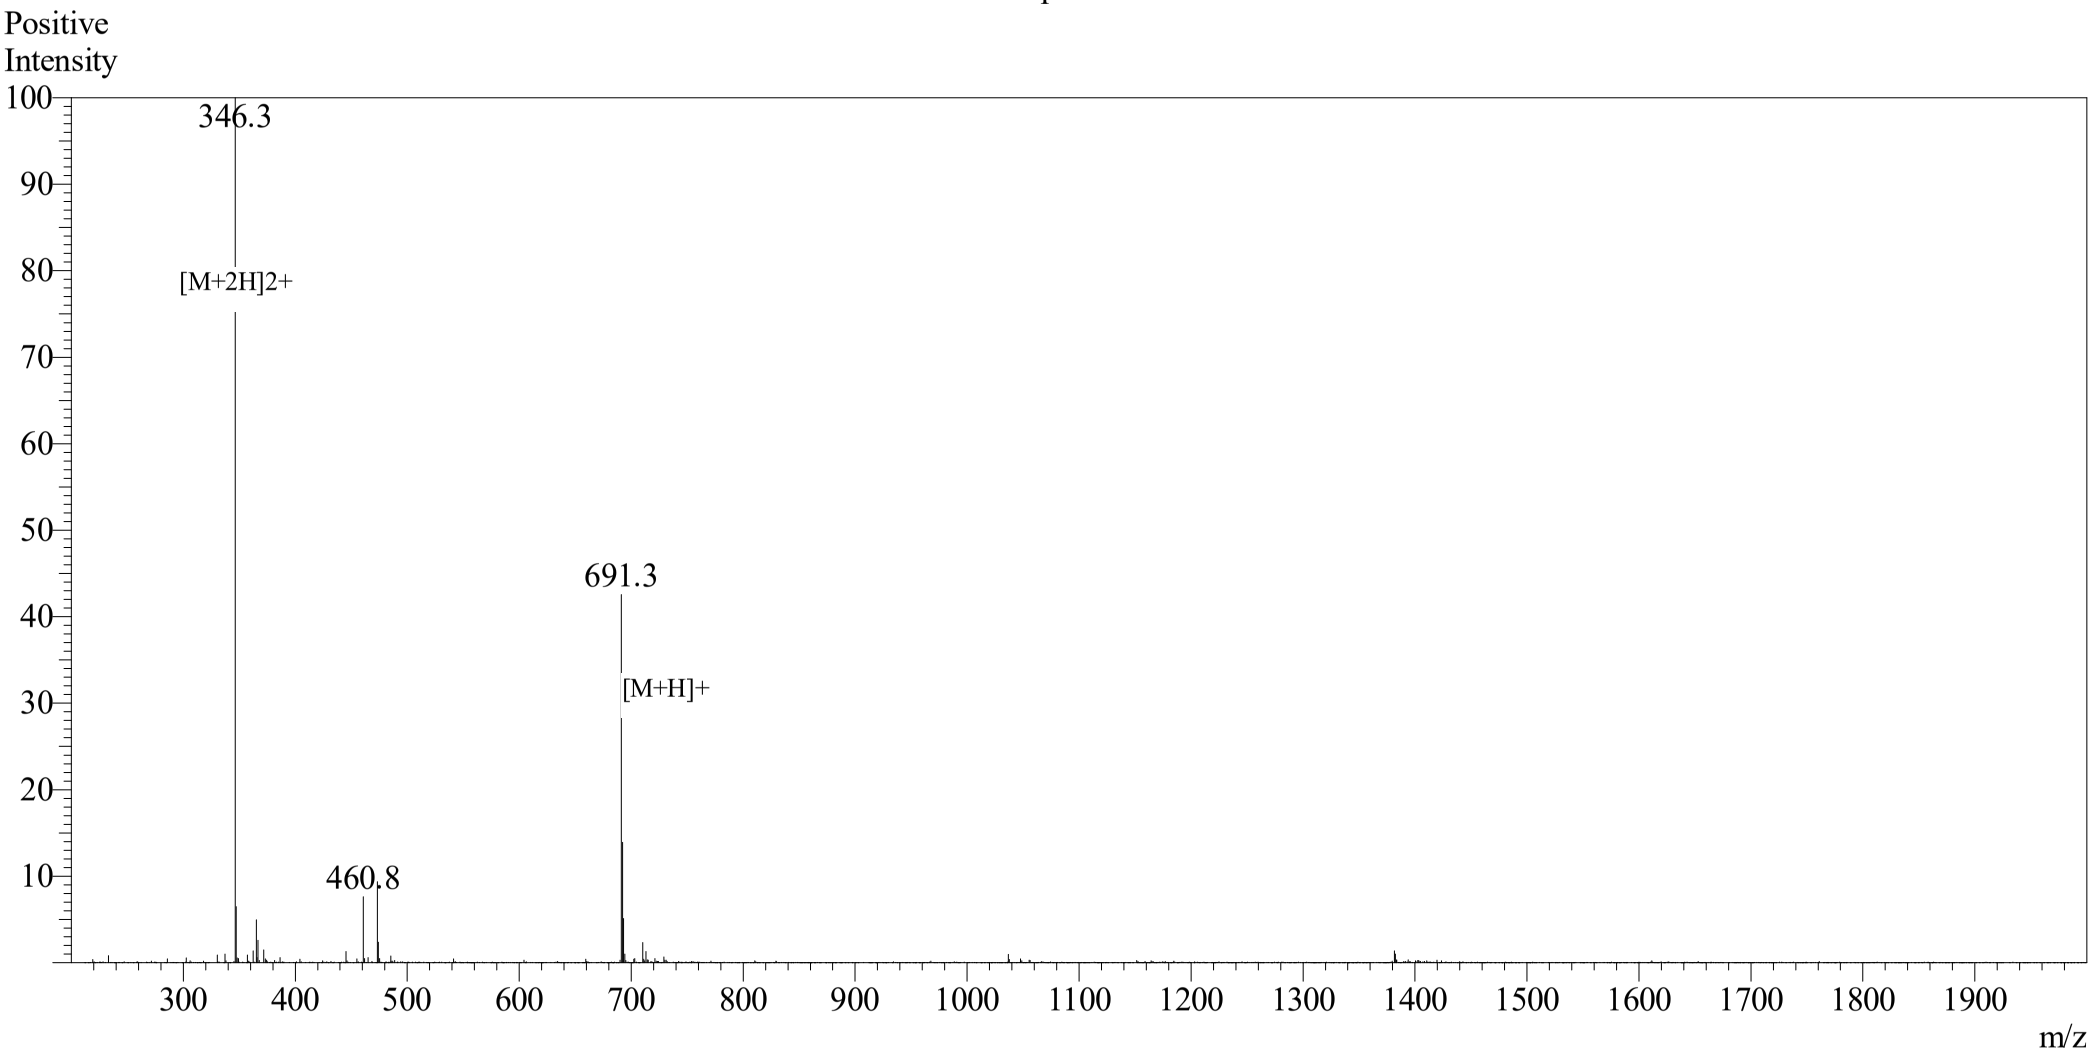

Sample Information	
User :	Gary
Month-Day Processed :	03/02/19
Time Processed :	01:06:02 PM
Injection Volume :	0.2
Sample Name :	GRGDSPC
Cat No. :	RP20283
Lot No. :	PE8721902
Theoretical MW :	690.73
Observed MW :	690.6

Interface	:ESI
Nebulizing Gas Flow	:1.5L/min
CDL Temp	:250
Block Temp	:200

Equipment	: GK11010007
Interface Bias	:+4.5kV
Drying Gas Flow	:5 L/min
T.Flow	:0.2ml/min
B.conc	:50%H2O/50%MeOH