

Sample Name :hgp100(25-33)
 Cat No. : RP20344
 Lot No. : E3603119K
 Time Processed : 21:00:44
 Month-Day-Year Processed : 11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 25.00 | Pumps | Pump B Conc. | 65 |
| 25.01 | Pumps | Pump B Conc. | 95 |
| 27.00 | Pumps | Pump B Conc. | 95 |
| 27.01 | Pumps | Pump B Conc. | 5 |
| 32.00 | Pumps | Pump B Conc. | 5 |
| 32.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

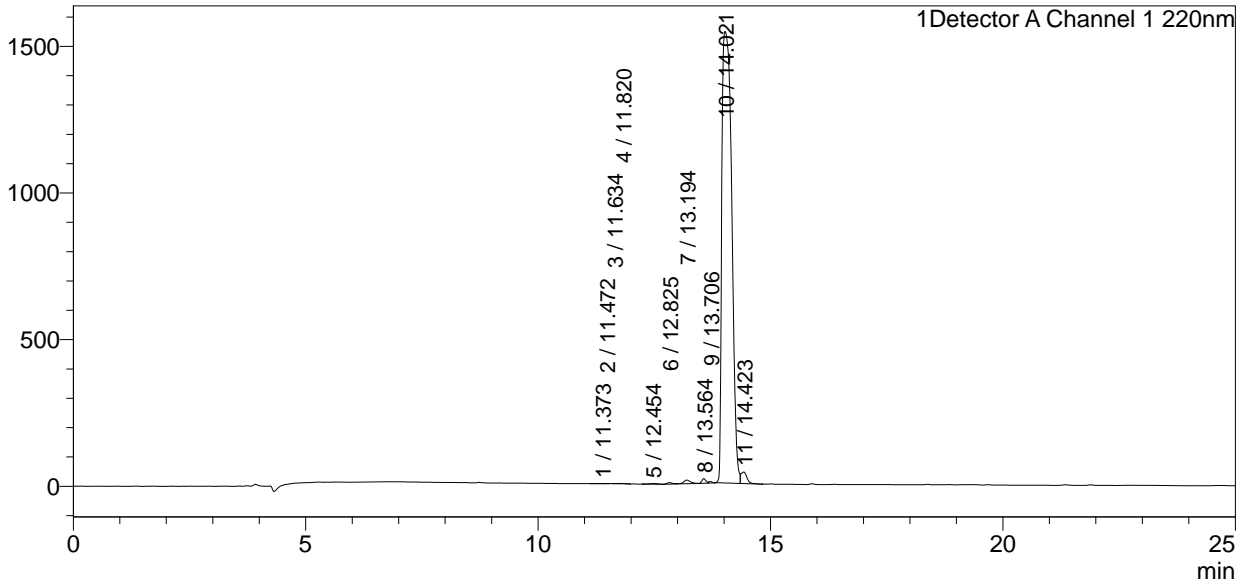

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 11.373 | 2188 | 204 | 0.009 |
| 2 | 11.472 | 1286 | 235 | 0.006 |
| 3 | 11.634 | 1070 | 184 | 0.005 |
| 4 | 11.820 | 4595 | 759 | 0.020 |
| 5 | 12.454 | 28124 | 2057 | 0.121 |
| 6 | 12.825 | 39541 | 4791 | 0.170 |
| 7 | 13.194 | 130008 | 12548 | 0.559 |
| 8 | 13.564 | 93853 | 15554 | 0.403 |
| 9 | 13.706 | 23500 | 4787 | 0.101 |
| 10 | 14.021 | 22604765 | 1539438 | 97.129 |
| 11 | 14.423 | 343901 | 39525 | 1.478 |
| Total | | 23272831 | 1620083 | 100.000 |