

Sample Name : HA Peptide
 Cat No.: RP11735
 Lot No.: E8808420E
 Time Processed : 11:26:03
 Month-Day-Year Processed : 05/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

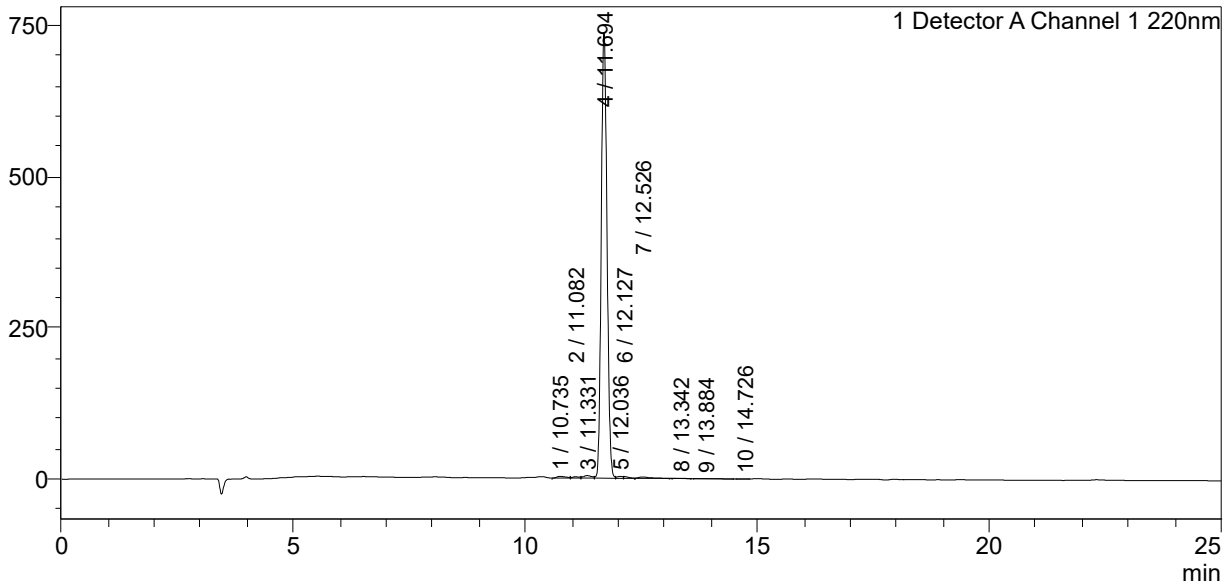

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.735	39165	2845	0.594
2	11.082	20814	2290	0.316
3	11.331	55729	4204	0.845
4	11.694	6361642	736816	96.454
5	12.036	21396	2968	0.324
6	12.127	26743	2853	0.405
7	12.526	44706	2351	0.678
8	13.342	7978	571	0.121
9	13.884	16223	579	0.246
10	14.726	1109	112	0.017
Total		6595505	755590	100.000