

Sample Name : Atrial Natriuretic Peptide (ANP) (1-28), human, porcine
 Cat No. : RP11927
 Lot No. : E1977621E
 Time Processed : 8:12:57 PM
 Month-Day-Year Processed : 06/01/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
65.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

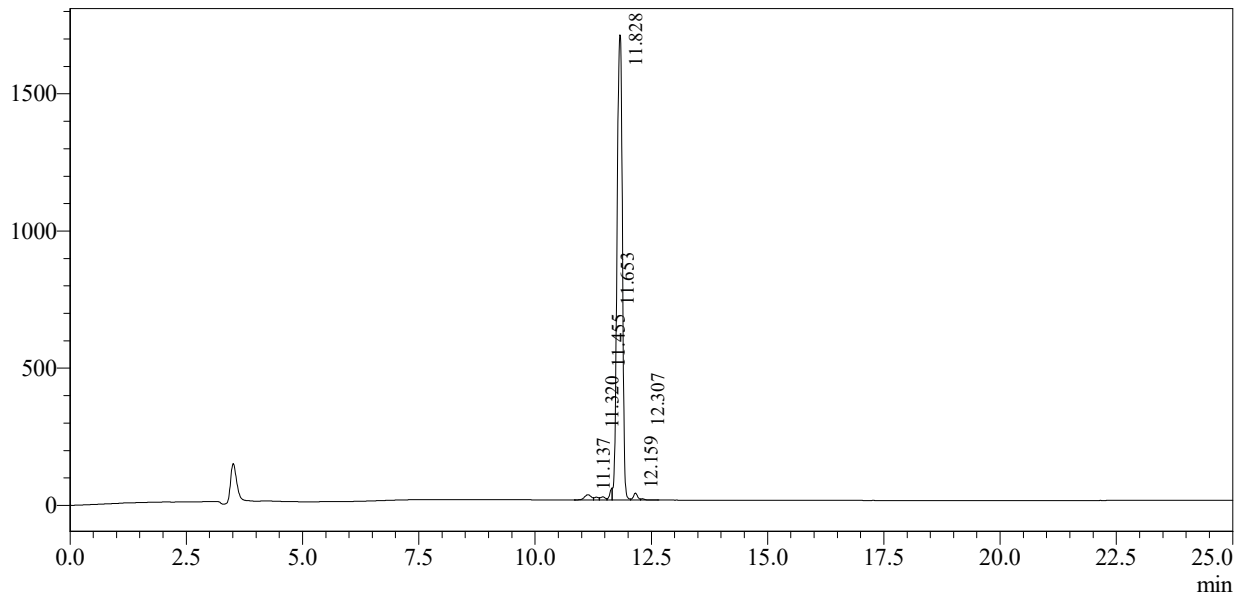

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.137	189989	18722	1.332
2	11.320	65674	9891	0.460
3	11.455	83135	11167	0.583
4	11.653	157492	42661	1.104
5	11.828	13588203	1695285	95.263
6	12.159	156267	25444	1.096
7	12.307	23102	4488	0.162
Total		14263862	1807658	100.000