

Sample Name :Angiotensin I, human  
 Cat No. :RP11251  
 Lot No. :PE1301905  
 Time Processed :22:59:19  
 Month-Day-Year Processed :05/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

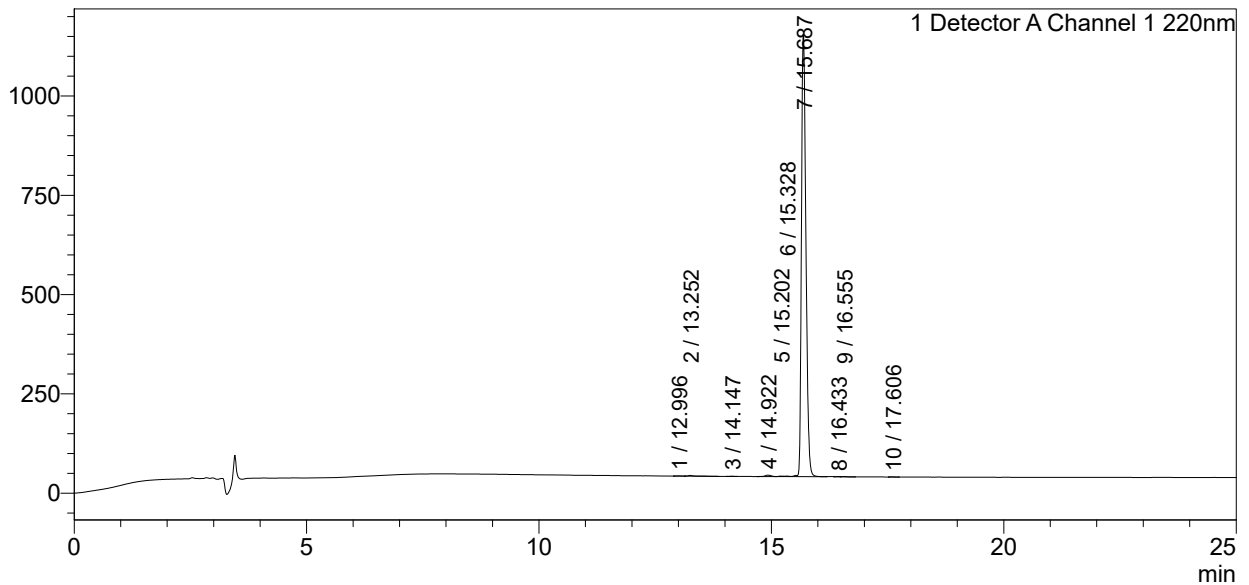

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.996	4016	558	0.053
2	13.252	20506	1968	0.272
3	14.147	2142	394	0.028
4	14.922	32167	3462	0.426
5	15.202	8069	1256	0.107
6	15.328	9654	1443	0.128
7	15.687	7457622	1113111	98.845
8	16.433	3156	529	0.042
9	16.555	5606	810	0.074
10	17.606	1808	349	0.024
Total		7544746	1123881	100.000