

Sample Name : γ - 2 - MSH (41 - 58), amide
 Cat. No. : RO20307
 Lot. No. : PE2471905
 Time Processed : 17:55:05
 Month-Day-Year Processed : 06/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.10	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

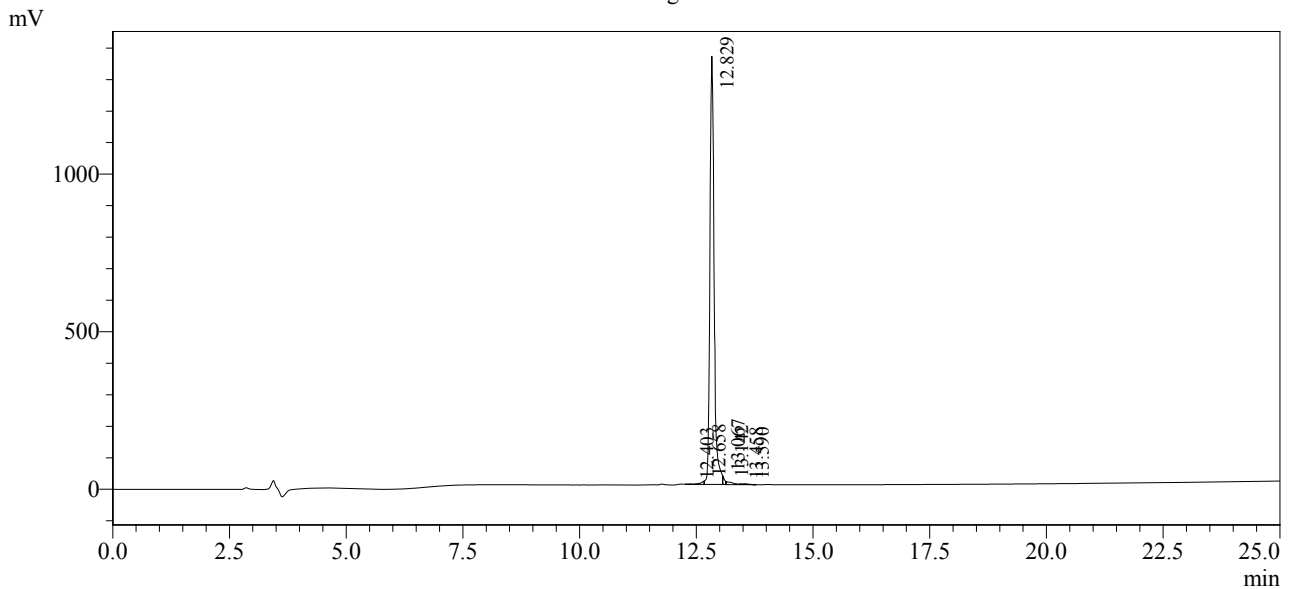

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.403	9572	1437	0.110
2	12.658	52982	10006	0.606
3	12.829	8503382	1358752	97.326
4	13.067	64303	27805	0.736
5	13.142	99539	8918	1.139
6	13.458	1367	182	0.016
7	13.590	5868	843	0.067
Total		8737013	1407942	100.000