Mass Spectrum

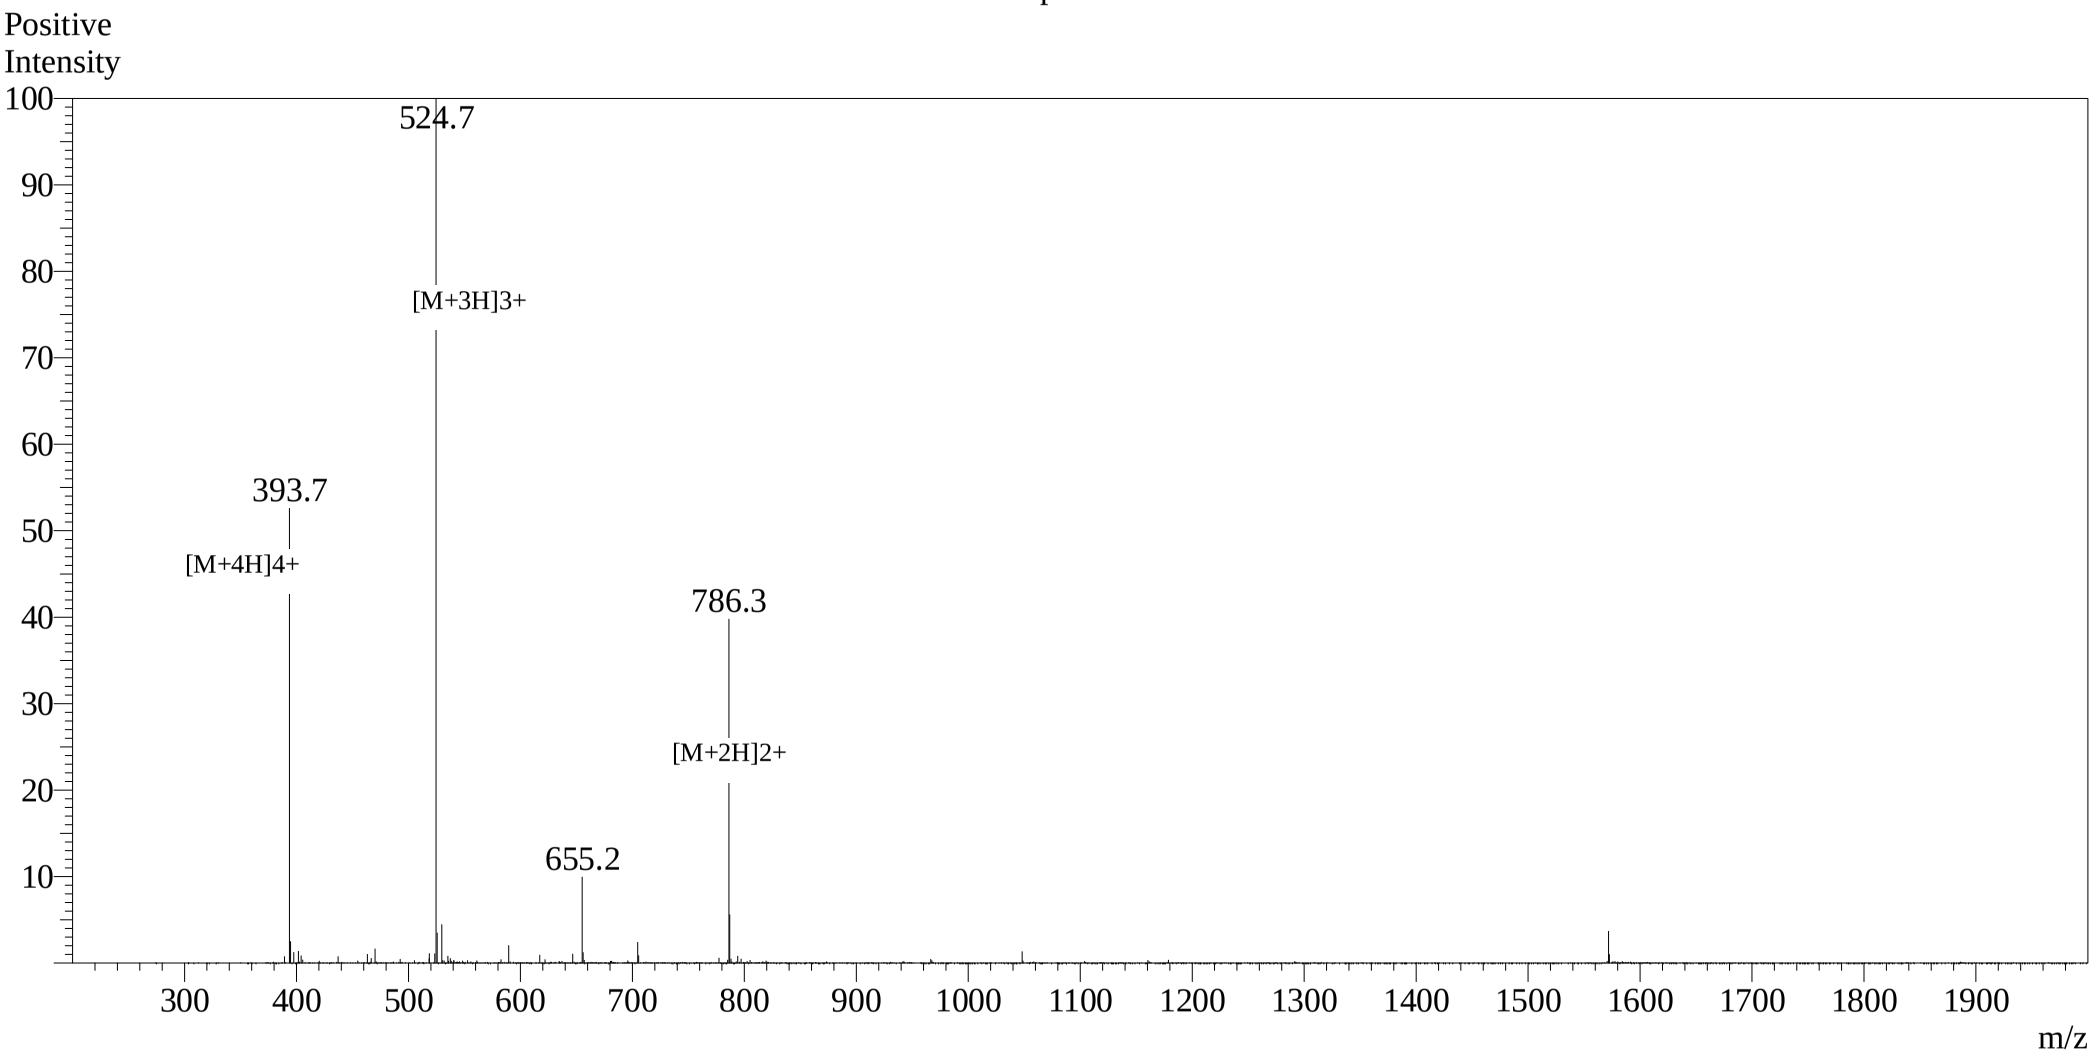

Sample Information	
User :	Gary
Month-Day Processed :	06/02/19
Time Processed :	9:51:23
Injection Volume :	0.3
Sample Name :	γ - 2 - MSH (41 - 58), amide
Cat No. :	RP20307
Lot No. :	PE2471905
Theoretical MW :	1570.78
Observed MW :	1571.1

Interface	:ESI
Nebulizing Gas Flow	:1.5L/min
CDL Temp	:250
Block Temp	:200

Equipment	: GK11010007
Interface Bias	:+4.5kV
Drying Gas Flow	:5 L/min
T.Flow	:0.2ml/min
B.conc	:50%H2O/50%MeOH