

Sample Name :Uty HY Peptide (246-254)

Cat No. : RP20261

Lot No. : E1284220J

Time Processed :5:35:37

Month-Day-Year Processed :10/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ20010139

<Chromatogram>

mV

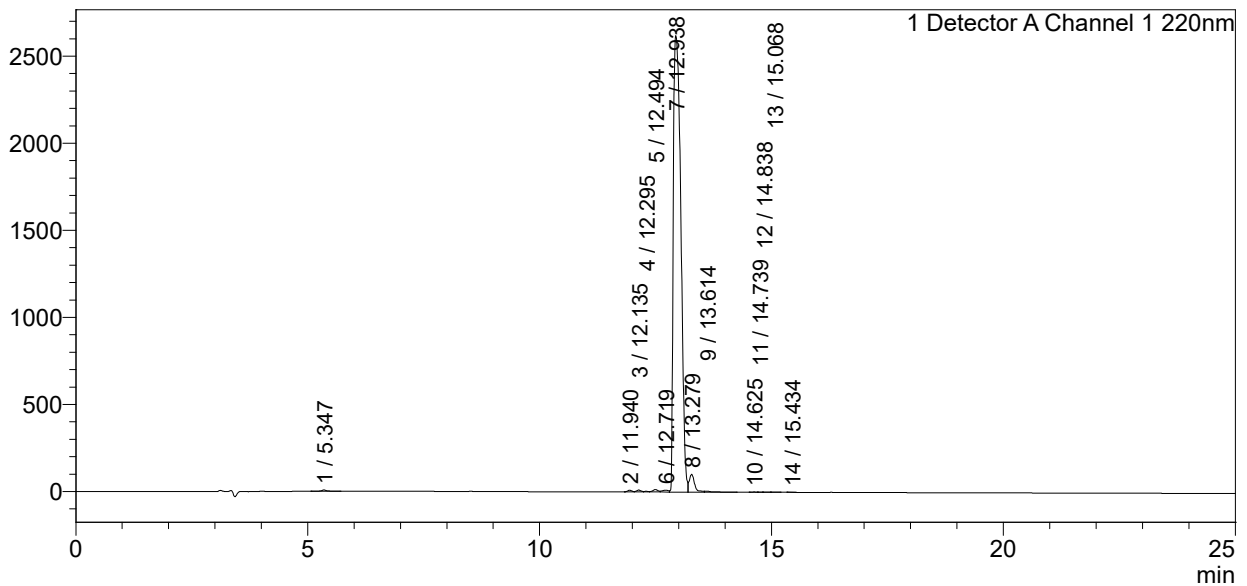

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.347	46720	6861	0.152
2	11.940	67202	10331	0.219
3	12.135	75099	10821	0.245
4	12.295	25857	3641	0.084
5	12.494	111683	14344	0.364
6	12.719	96922	10600	0.316
7	12.938	29393847	2621097	95.719
8	13.279	811125	101800	2.641
9	13.614	58229	6023	0.190
10	14.625	7550	1175	0.025
11	14.739	4400	746	0.014
12	14.838	3487	645	0.011
13	15.068	1658	283	0.005
14	15.434	4645	818	0.015
Total		30708425	2789186	100.000