

Sample Name : Cys-TAT(47-57)

Cat. No. :RP20343

Lot. No. :PE4021711

Pump A : 0.065% trifluoroacetic in 100% water

Pump B : 0.05% trifluoroacetic in 100% acetonitrile

Total Flow:1 ml/min


Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

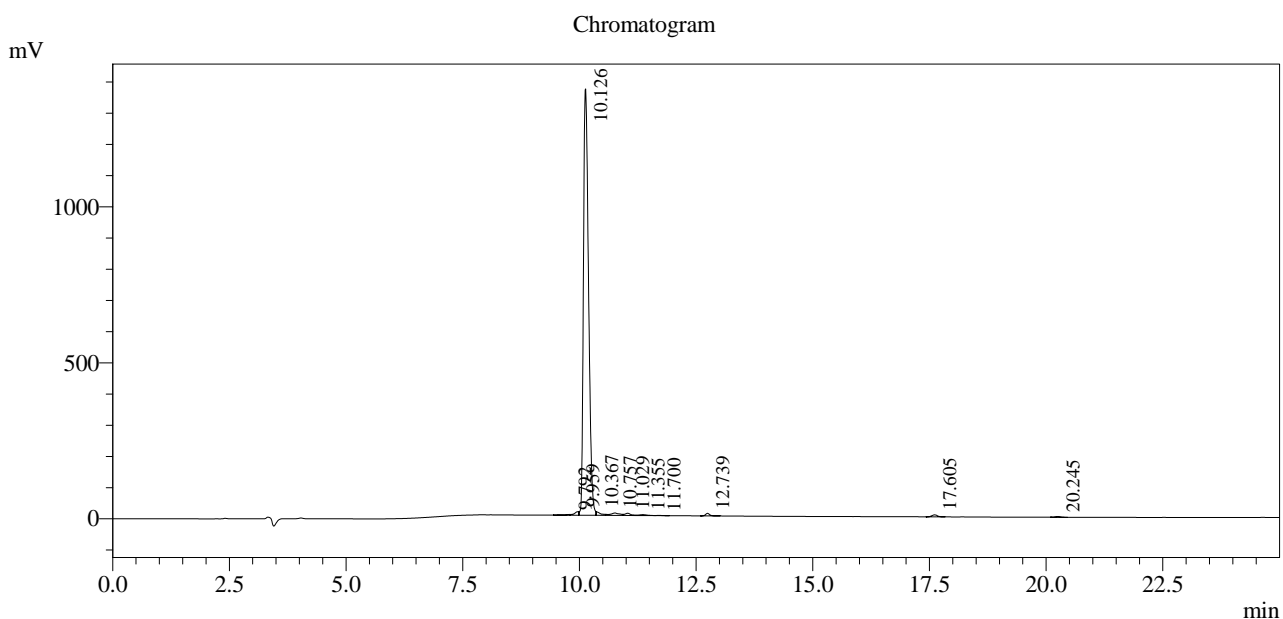

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.792	16595	2107	0.153
2	9.959	75271	11064	0.695
3	10.126	10340176	1366569	95.430
4	10.367	71894	11186	0.664
5	10.757	107848	7865	0.995
6	11.029	63750	7192	0.588
7	11.355	36446	2819	0.336
8	11.700	5749	892	0.053
9	12.739	49498	8086	0.457
10	17.605	55043	6550	0.508
11	20.245	13082	1885	0.121
Total		10835353	1426217	100.000