

Sample Name : Secretin, canine
 Cat No : RP12943
 Lot No : E0637321A
 Time Processed : 9:05:08
 Month-Day-Year Processed : 02/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

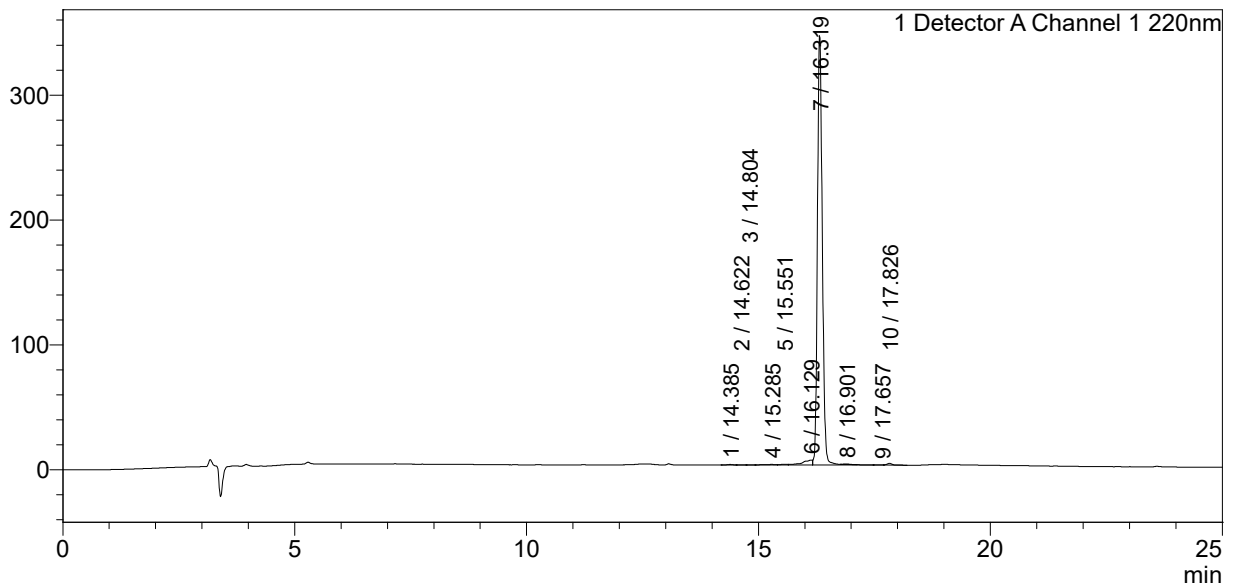

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.385	3407	409	0.131
2	14.622	1033	121	0.040
3	14.804	1049	133	0.040
4	15.285	7426	459	0.285
5	15.551	6319	604	0.243
6	16.129	58407	3986	2.241
7	16.319	2511468	343816	96.378
8	16.901	3702	383	0.142
9	17.657	1110	139	0.043
10	17.826	11925	1437	0.458
Total		2605847	351487	100.000