

Sample Name :Glucagon (19-29), human  
 Cat No: RP10770  
 Lot No : E6356321G  
 Time Processed :1:10:17 AM  
 Month-Day-Year Processed :07/25/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

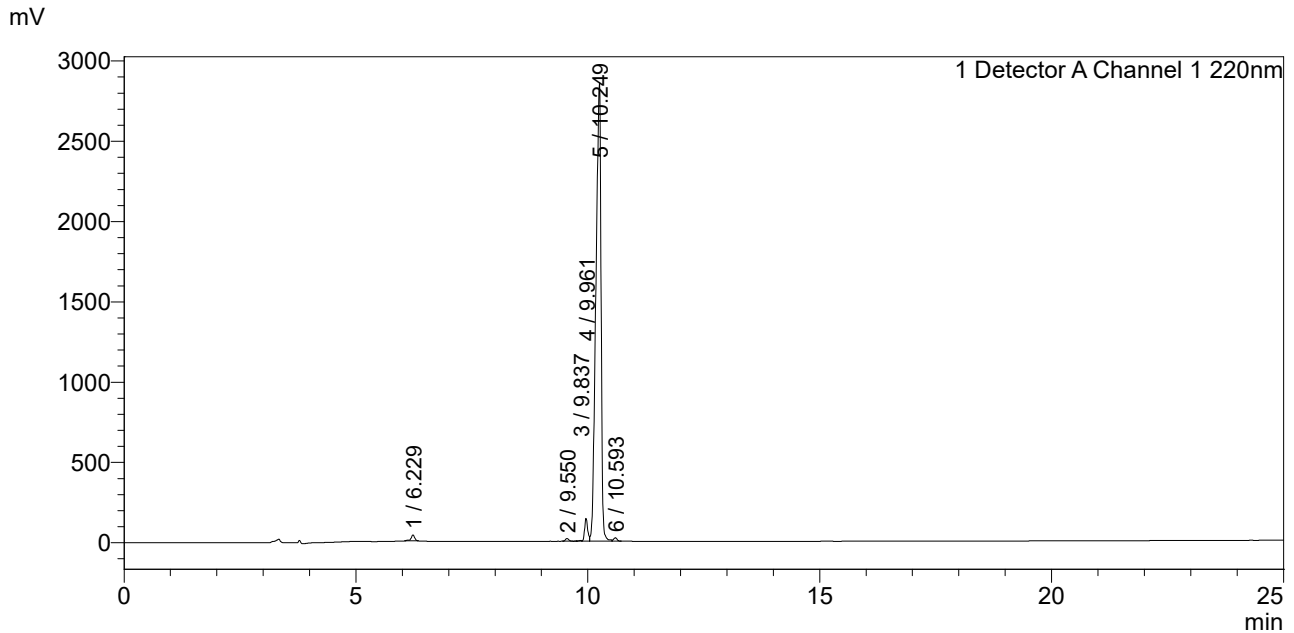

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.229	193225	35479	0.843
2	9.550	76385	16092	0.333
3	9.837	18070	3805	0.079
4	9.961	656260	142040	2.864
5	10.249	21864607	2855713	95.416
6	10.593	106570	21496	0.465
Total		22915116	3074625	100.000