

Sample Name :Substance P
 Cat No. :RP10178
 Lot No. :E1399819G
 Time Processed :23:23:58
 Month-Day-Year Processed :07/26/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

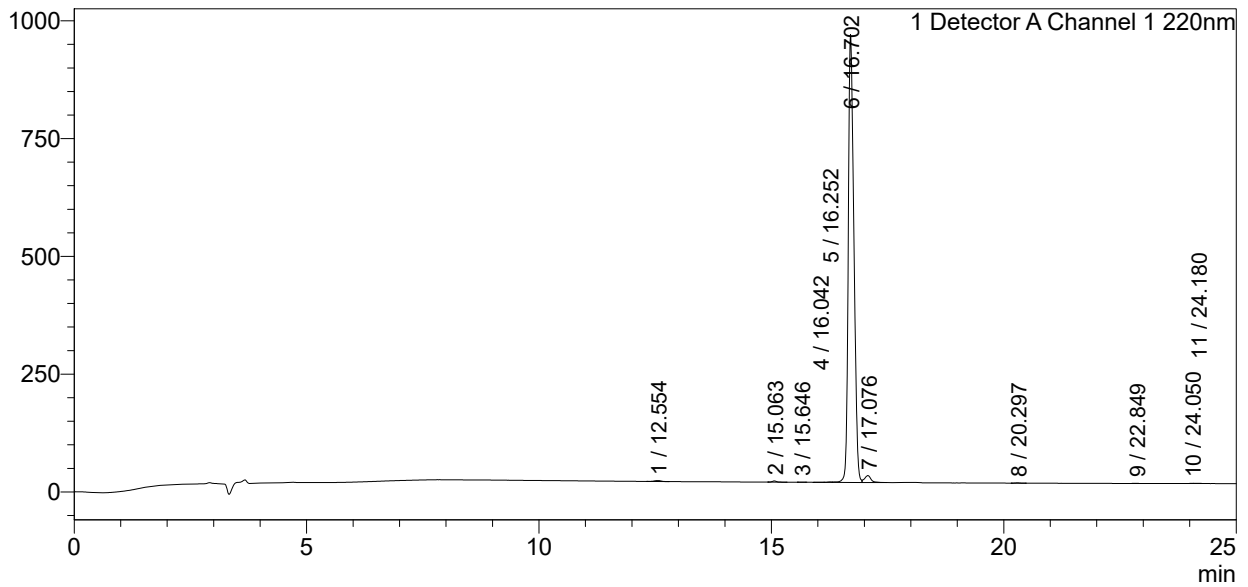

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.554	19869	2018	0.244
2	15.063	17473	2630	0.214
3	15.646	1133	227	0.014
4	16.042	1749	250	0.021
5	16.252	6133	925	0.075
6	16.702	7950147	951000	97.515
7	17.076	141709	14694	1.738
8	20.297	3480	567	0.043
9	22.849	2043	194	0.025
10	24.050	3101	455	0.038
11	24.180	5916	578	0.073
Total		8152752	973539	100.000