

Sample Name : Neurotensin
 Cat. No. : RP10439
 Lot. No. : PE9231812
 Time Processed : 20:15:11
 Month-Day-Year Processed : 12/14/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

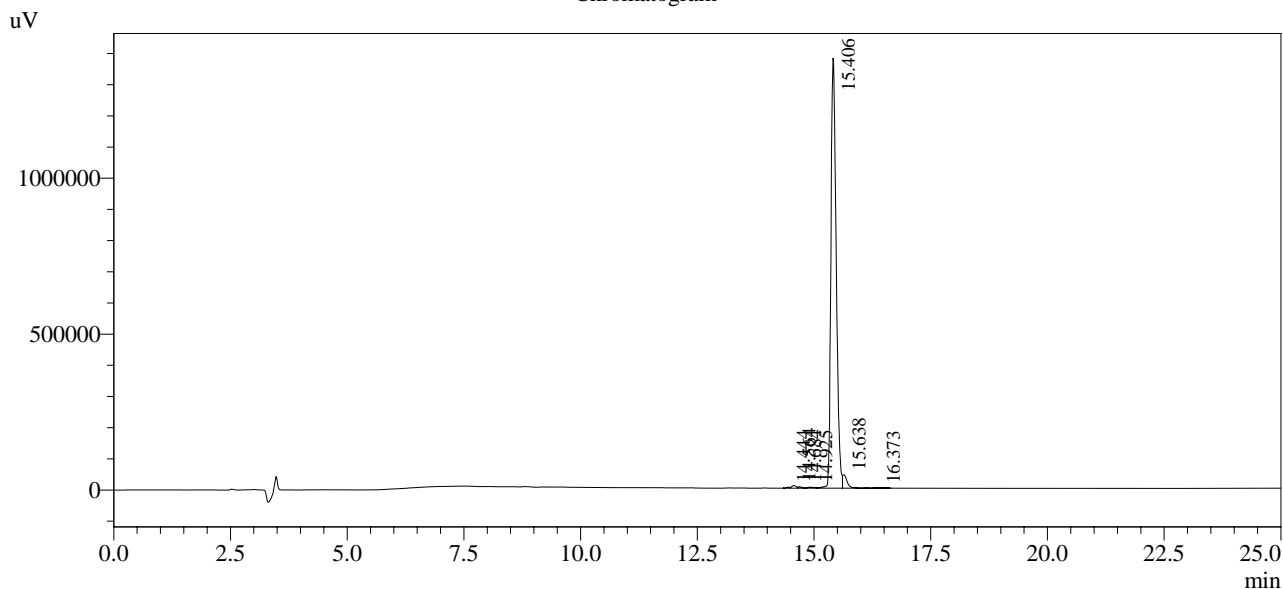

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.444	15684	3078	0.139
2	14.564	56872	8608	0.505
3	14.684	24480	3974	0.217
4	14.925	33206	3394	0.295
5	15.406	10845886	1378960	96.218
6	15.638	292321	42934	2.593
7	16.373	3805	344	0.034
Total		11272253	1441292	100.000