


Mass Spectrum

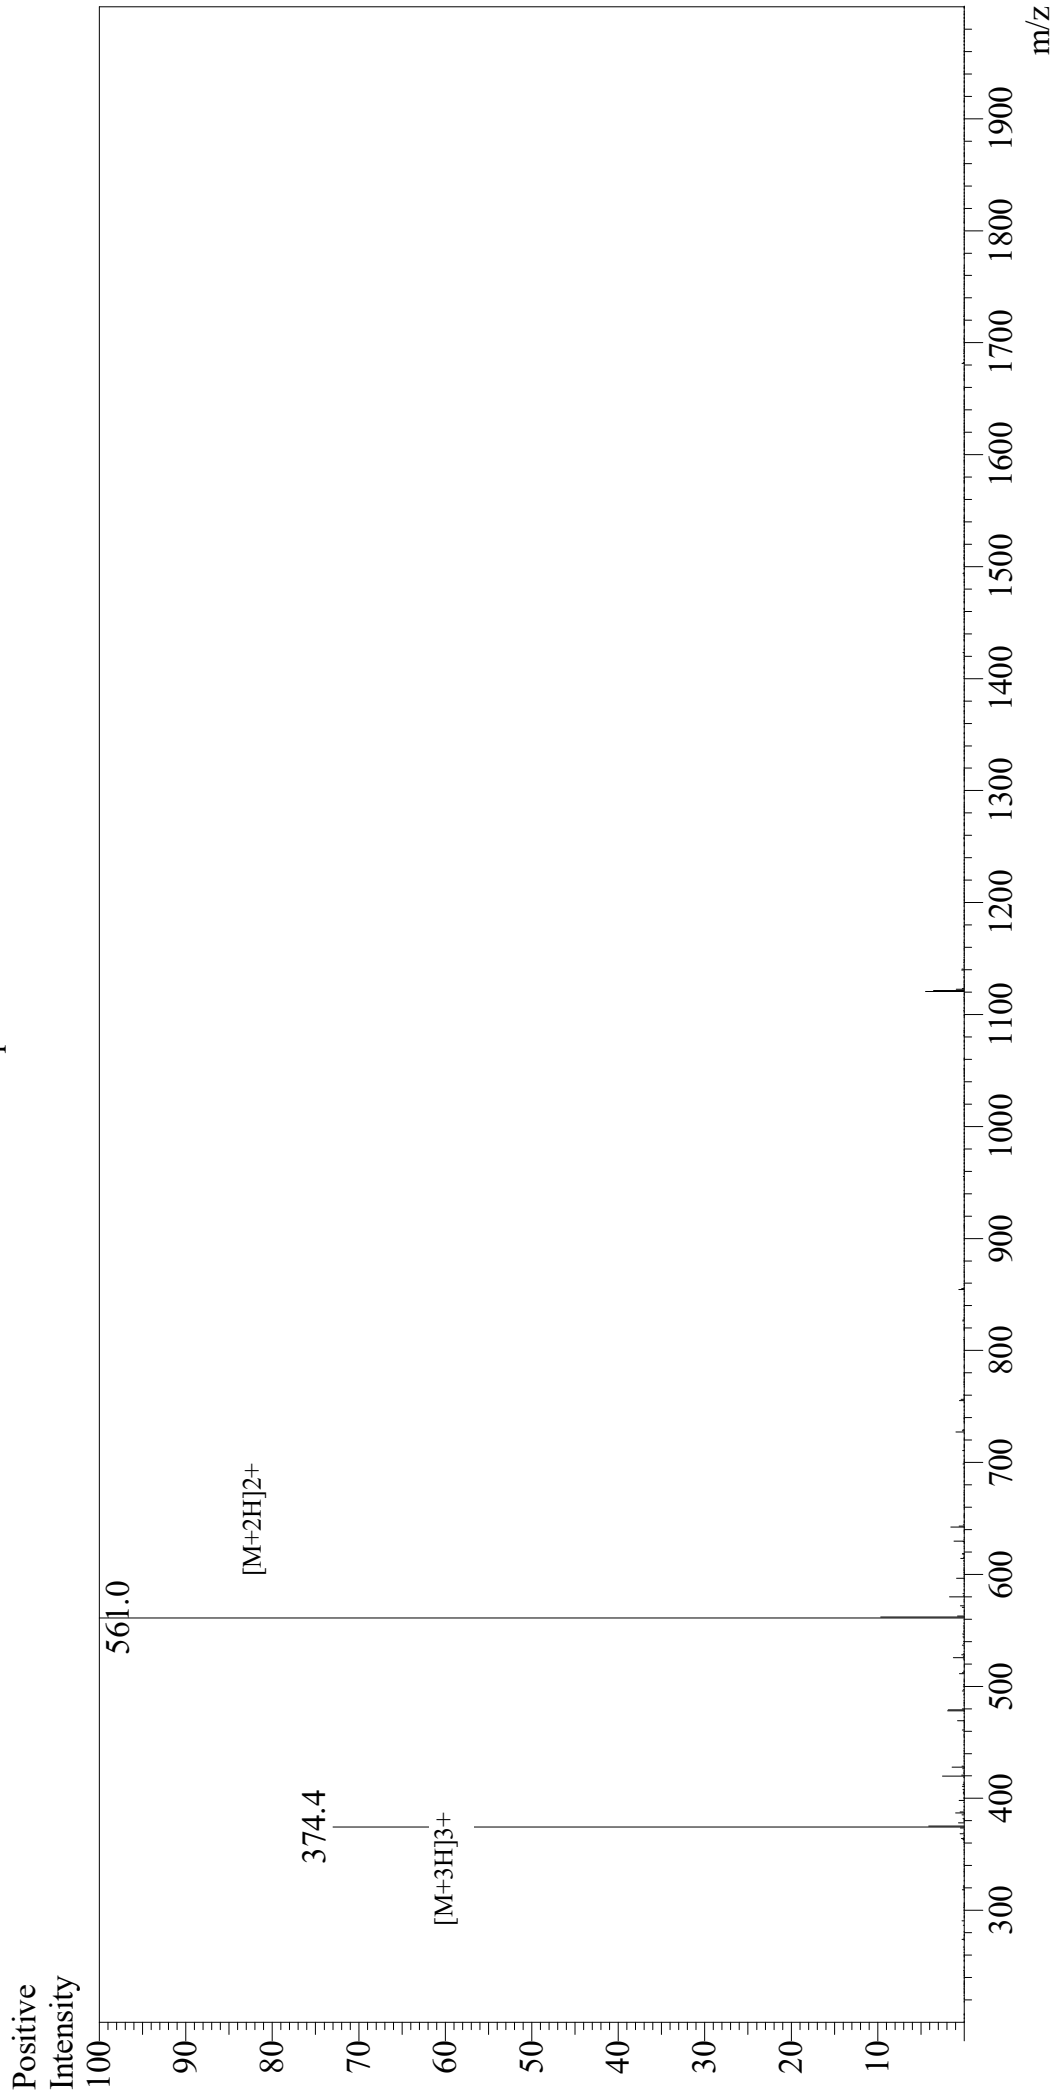

Sample Information

User : Gary
Month-Day Processed : 04/08/20
Time Processed : 09:04:49 AM
Injection Volume : 0.3
Sample Name : Human Papillomavirus (HPV) E7 protein (49 - 57)
Cat No. : RP20249
Lot No. : E0403320D
Theoretical MW : 1120.27
Observed MW : 1120.0

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200