

Sample Name:Oxytocin  
 Cat No. : RP10407  
 Lot No. :4396421E  
 Time Processed : 15:43:33  
 Month-Day-Year Processed : 06/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

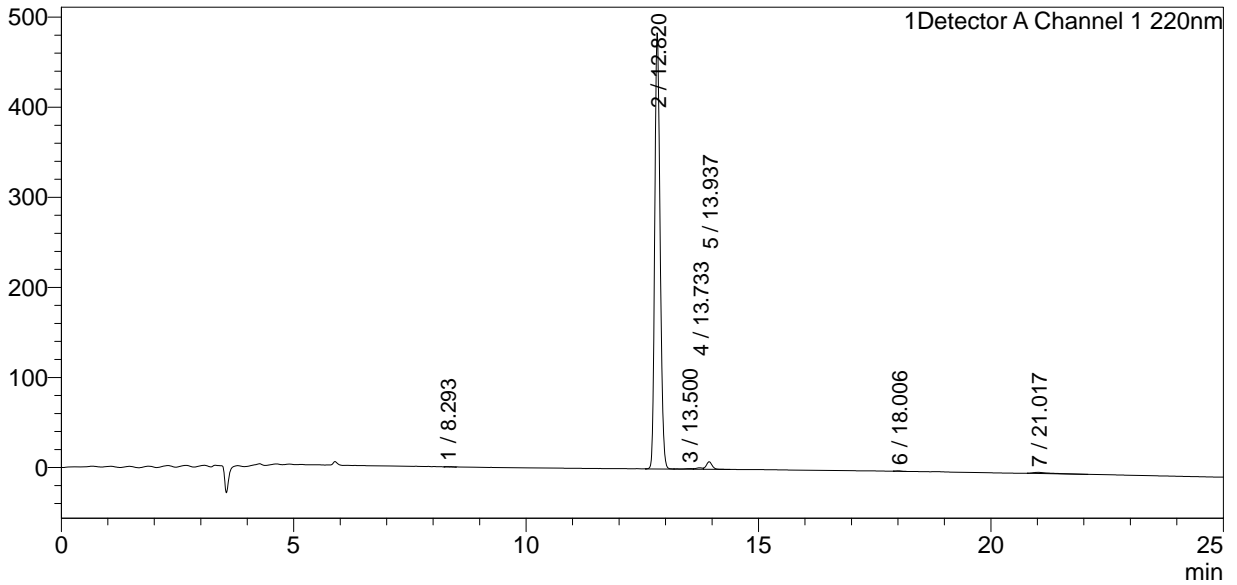

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.293	2366	276	0.059
2	12.820	3883852	478614	96.538
3	13.500	10484	686	0.261
4	13.733	15758	1596	0.392
5	13.937	72183	8333	1.794
6	18.006	3199	497	0.080
7	21.017	35292	1232	0.877
Total		4023134	491235	100.000