

Sample Name :Neurotensin
Cat. No. : RP10439
Lot. No.: E1095319G
Time Processed :10:28:31
Month-Day-Year Processed : 07/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

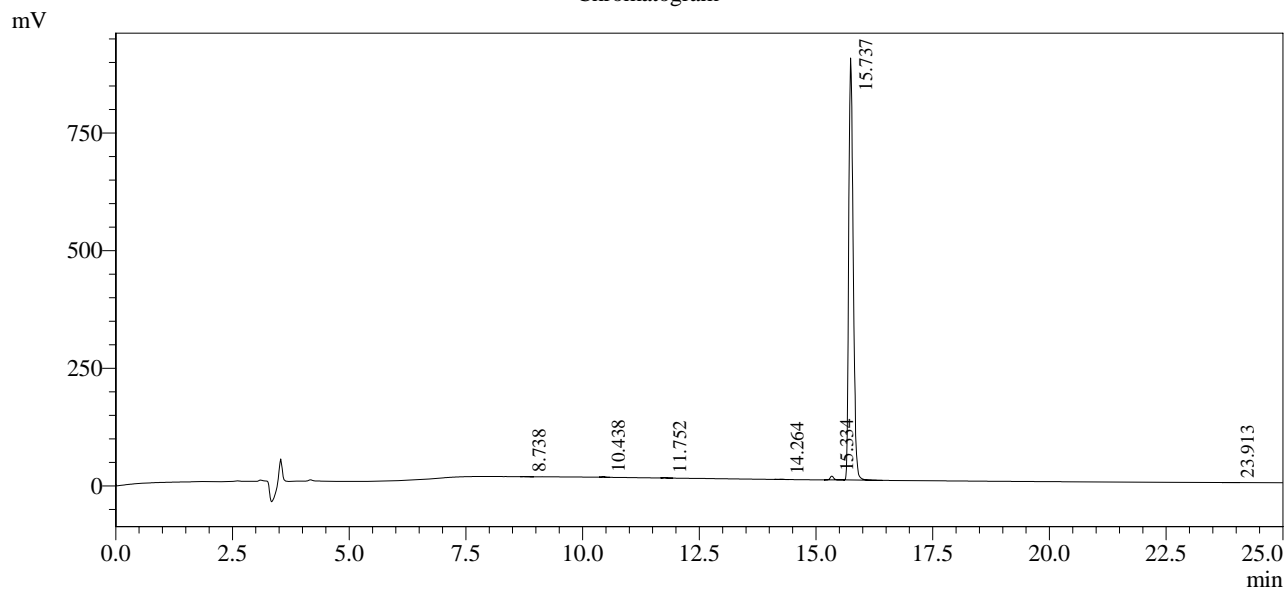

1 Det.A Ch1 / 220nm
Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.738	1381	274	0.023
2	10.438	5925	1273	0.098
3	11.752	4017	833	0.066
4	14.264	3734	519	0.062
5	15.334	43074	7950	0.711
6	15.737	5999973	896991	98.992
7	23.913	2985	368	0.049
Total		6061090	908206	100.000