


Mass Spectrum

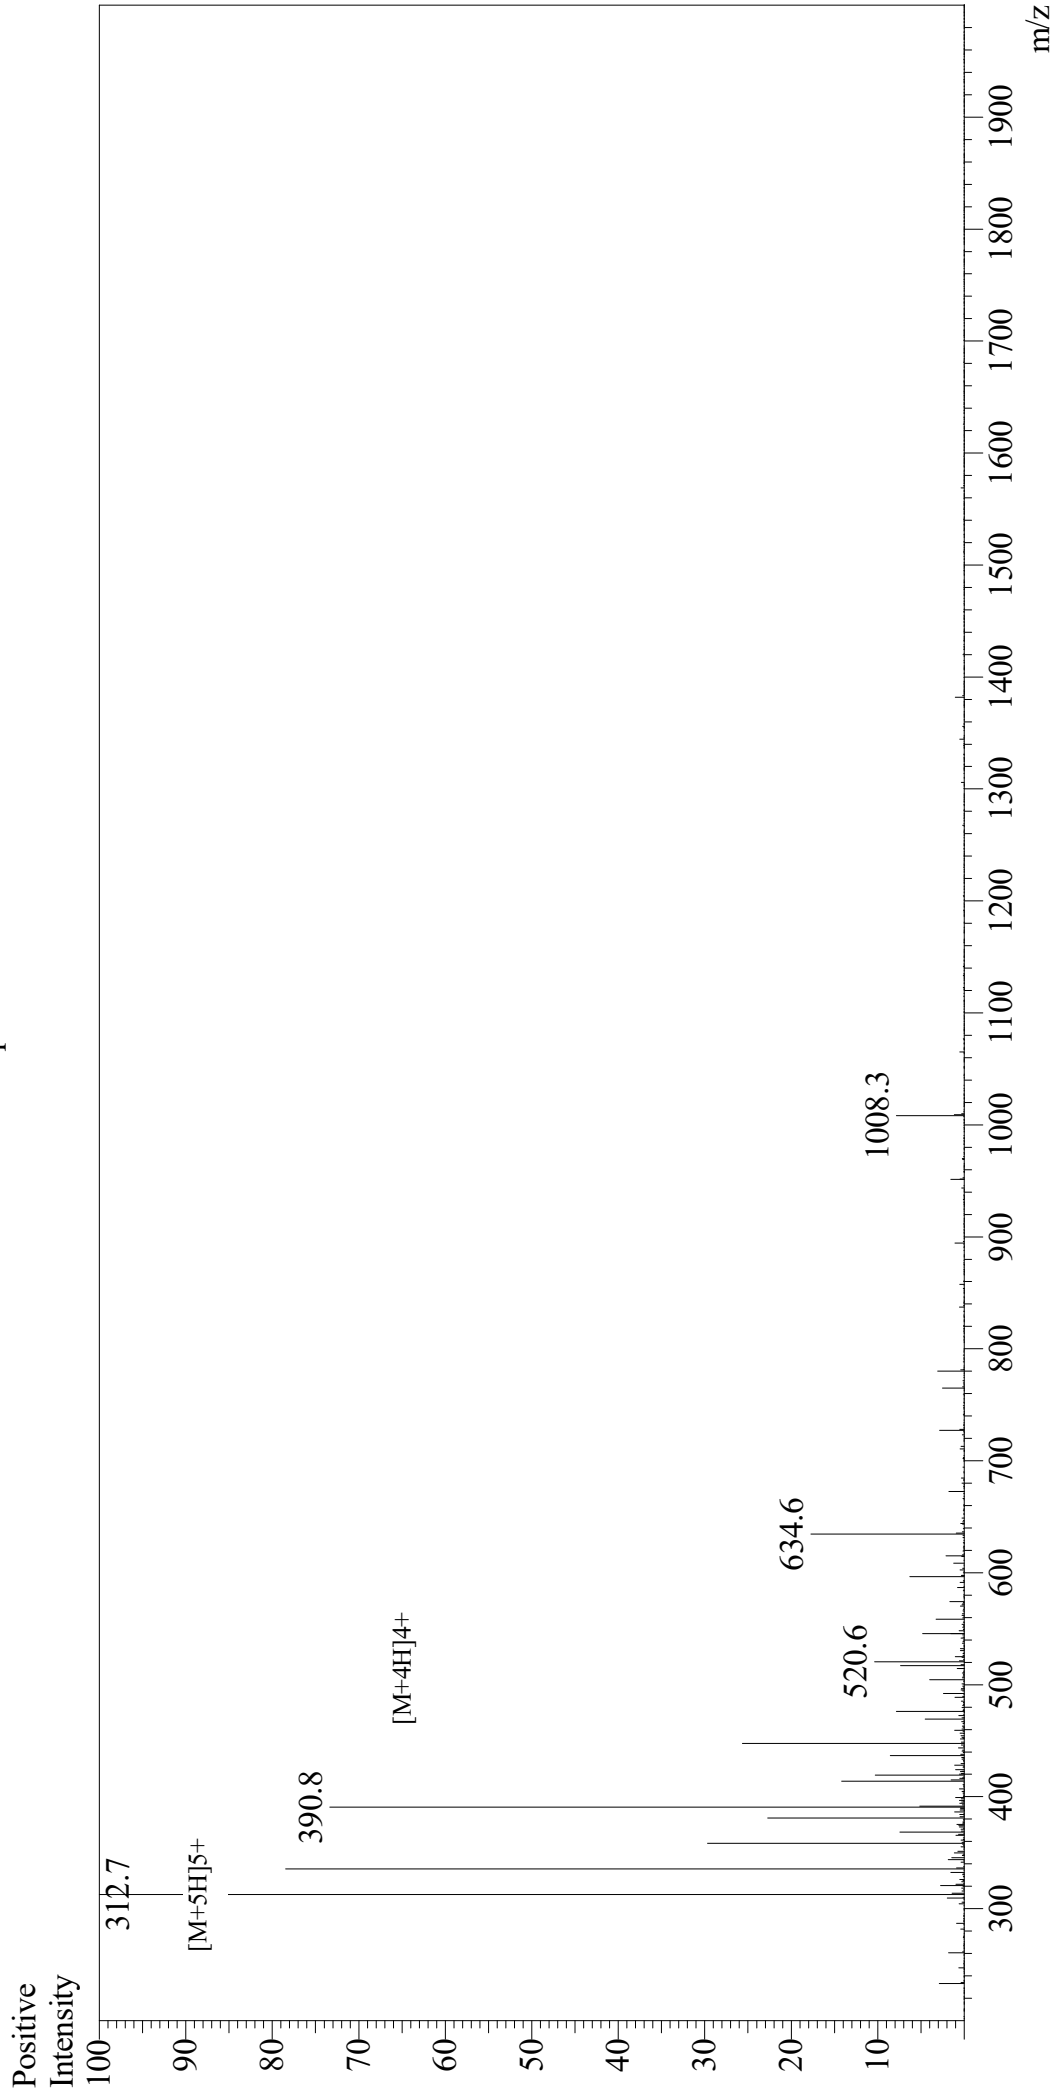

Sample Information

User : Gary
Month-Day Processed : 09/19/19
Time Processed : 08:56:12 PM
Injection Volume : 0.4
Sample Name : TAT
Cat No. : RP12784
Lot No. : E4890619I
Theoretical MW : 1558.85
Observed MW : 1558.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH