

Sample Name : Influenza Hemagglutinin (307-319)
 Cat No. : RP20087
 Lot No. : E9596019L
 Time Processed : 7:48:43
 Month-Day-Year Processed : 12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

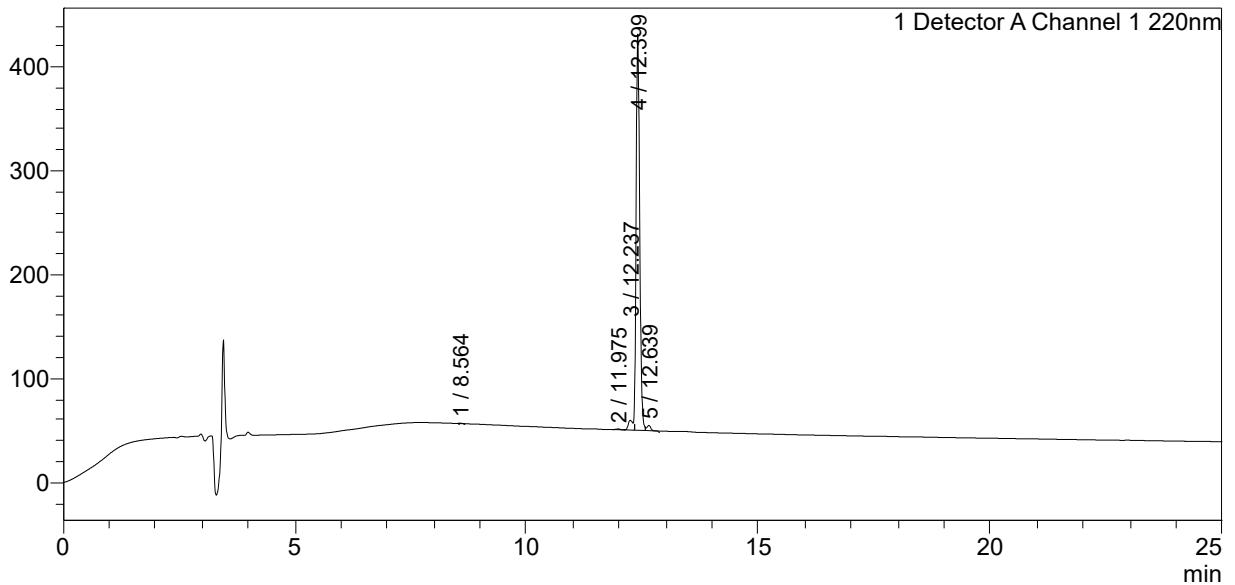

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.564	1690	391	0.078
2	11.975	4389	856	0.204
3	12.237	59884	9360	2.780
4	12.399	2061885	381592	95.709
5	12.639	26470	5065	1.229
Total		2154318	397263	100.000