

Sample Name :Gastrin-Releasing Peptide, human  
 Cat No. :RP10791  
 Lot No. :E5058820J  
 Time Processed :11:47:15  
 Month-Day-Year Processed :10/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

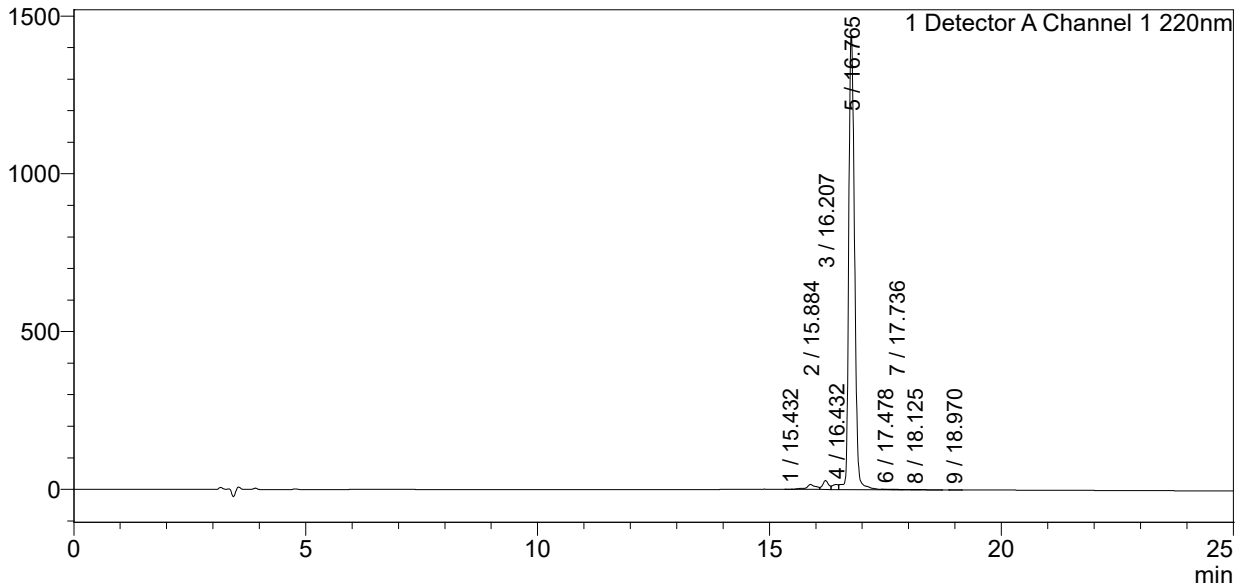

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.432	1442	233	0.011
2	15.884	227254	15601	1.724
3	16.207	250595	28477	1.901
4	16.432	141839	15736	1.076
5	16.765	12552593	1438768	95.215
6	17.478	2491	173	0.019
7	17.736	3627	524	0.028
8	18.125	1320	238	0.010
9	18.970	2197	301	0.017
Total		13183357	1500051	100.000