

Sample Name :Speract
 Cat No. :RP10620
 Lot No. :E4744419I
 Time Processed :15:03:52
 Month-Day-Year Processed :09/20/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

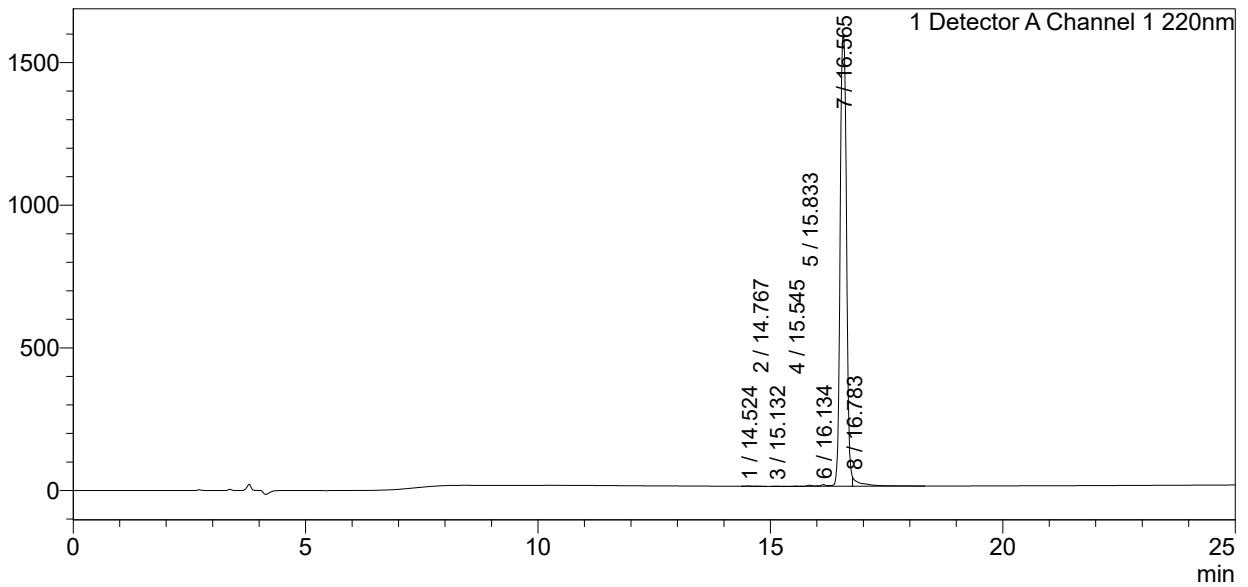

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.524	10115	1505	0.066
2	14.767	1408	186	0.009
3	15.132	2762	404	0.018
4	15.545	6192	852	0.040
5	15.833	34833	3727	0.226
6	16.134	44388	5527	0.288
7	16.565	14937786	1578830	97.035
8	16.783	356758	28102	2.317
Total		15394243	1619133	100.000