

Sample Name :Osteogenic Growth Peptide, OGP  
 Cat. No. : RP20311  
 Lot. No. :E2445919K  
 Time Processed :4:24:23  
 Month-Day-Year Processed :11/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

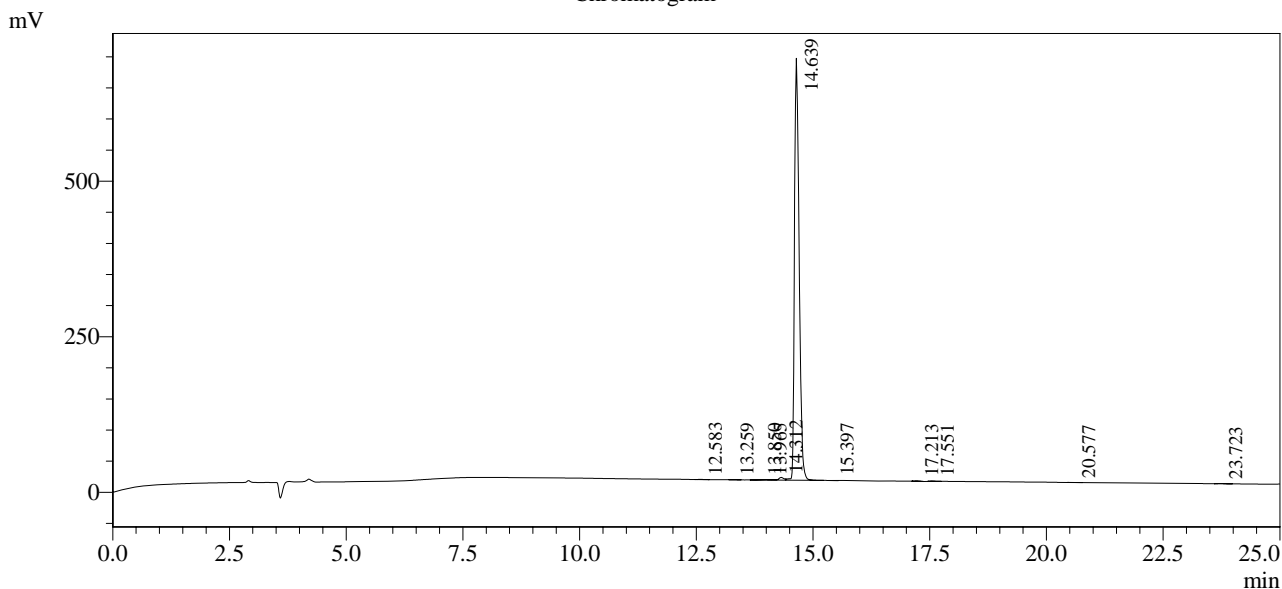

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.583	2054	298	0.043
2	13.259	2640	315	0.055
3	13.850	2005	262	0.042
4	13.965	5880	648	0.123
5	14.312	34030	4385	0.712
6	14.639	4721526	678299	98.760
7	15.397	3103	598	0.065
8	17.213	1919	351	0.040
9	17.551	2836	440	0.059
10	20.577	1047	114	0.022
11	23.723	3755	464	0.079
Total		4780793	686174	100.000