

Sample Name : hgp100(25-33)
 Cat. No. : RP20344
 Lot. No. : PE3531611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

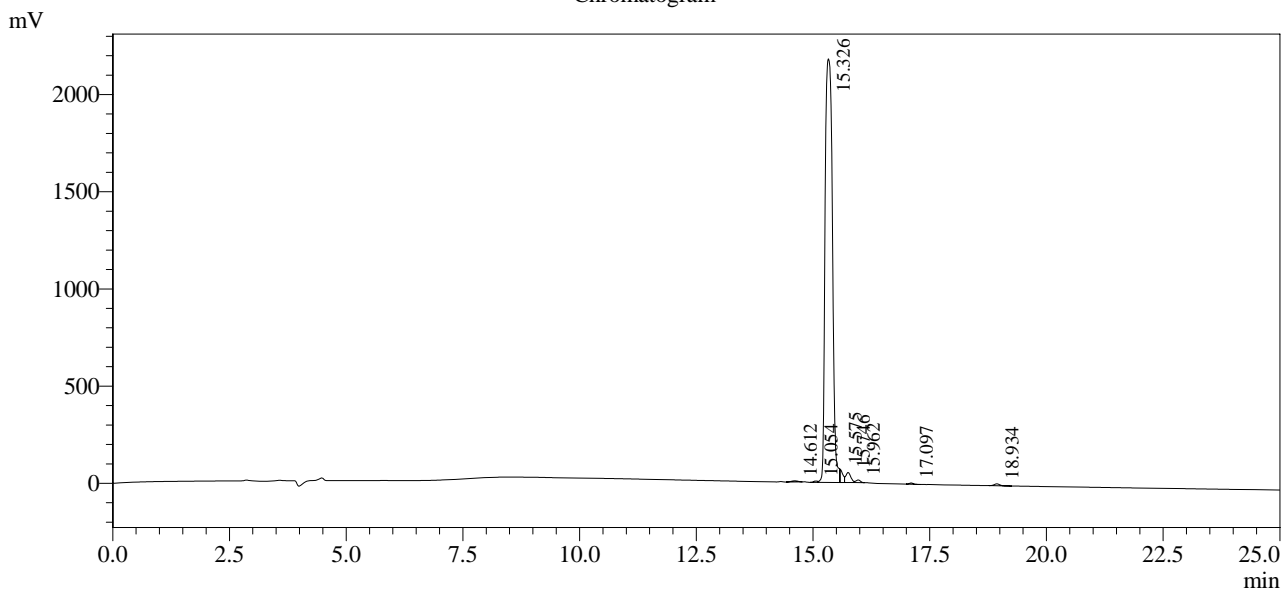

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.612	59162	6061	0.239
2	15.054	42586	7668	0.172
3	15.326	23739263	2179420	96.019
4	15.575	283742	70310	1.148
5	15.746	390426	51831	1.579
6	15.962	91575	13965	0.370
7	17.097	37410	6783	0.151
8	18.934	79392	9747	0.321
Total		24723556	2345786	100.000