


# Mass Spectrum

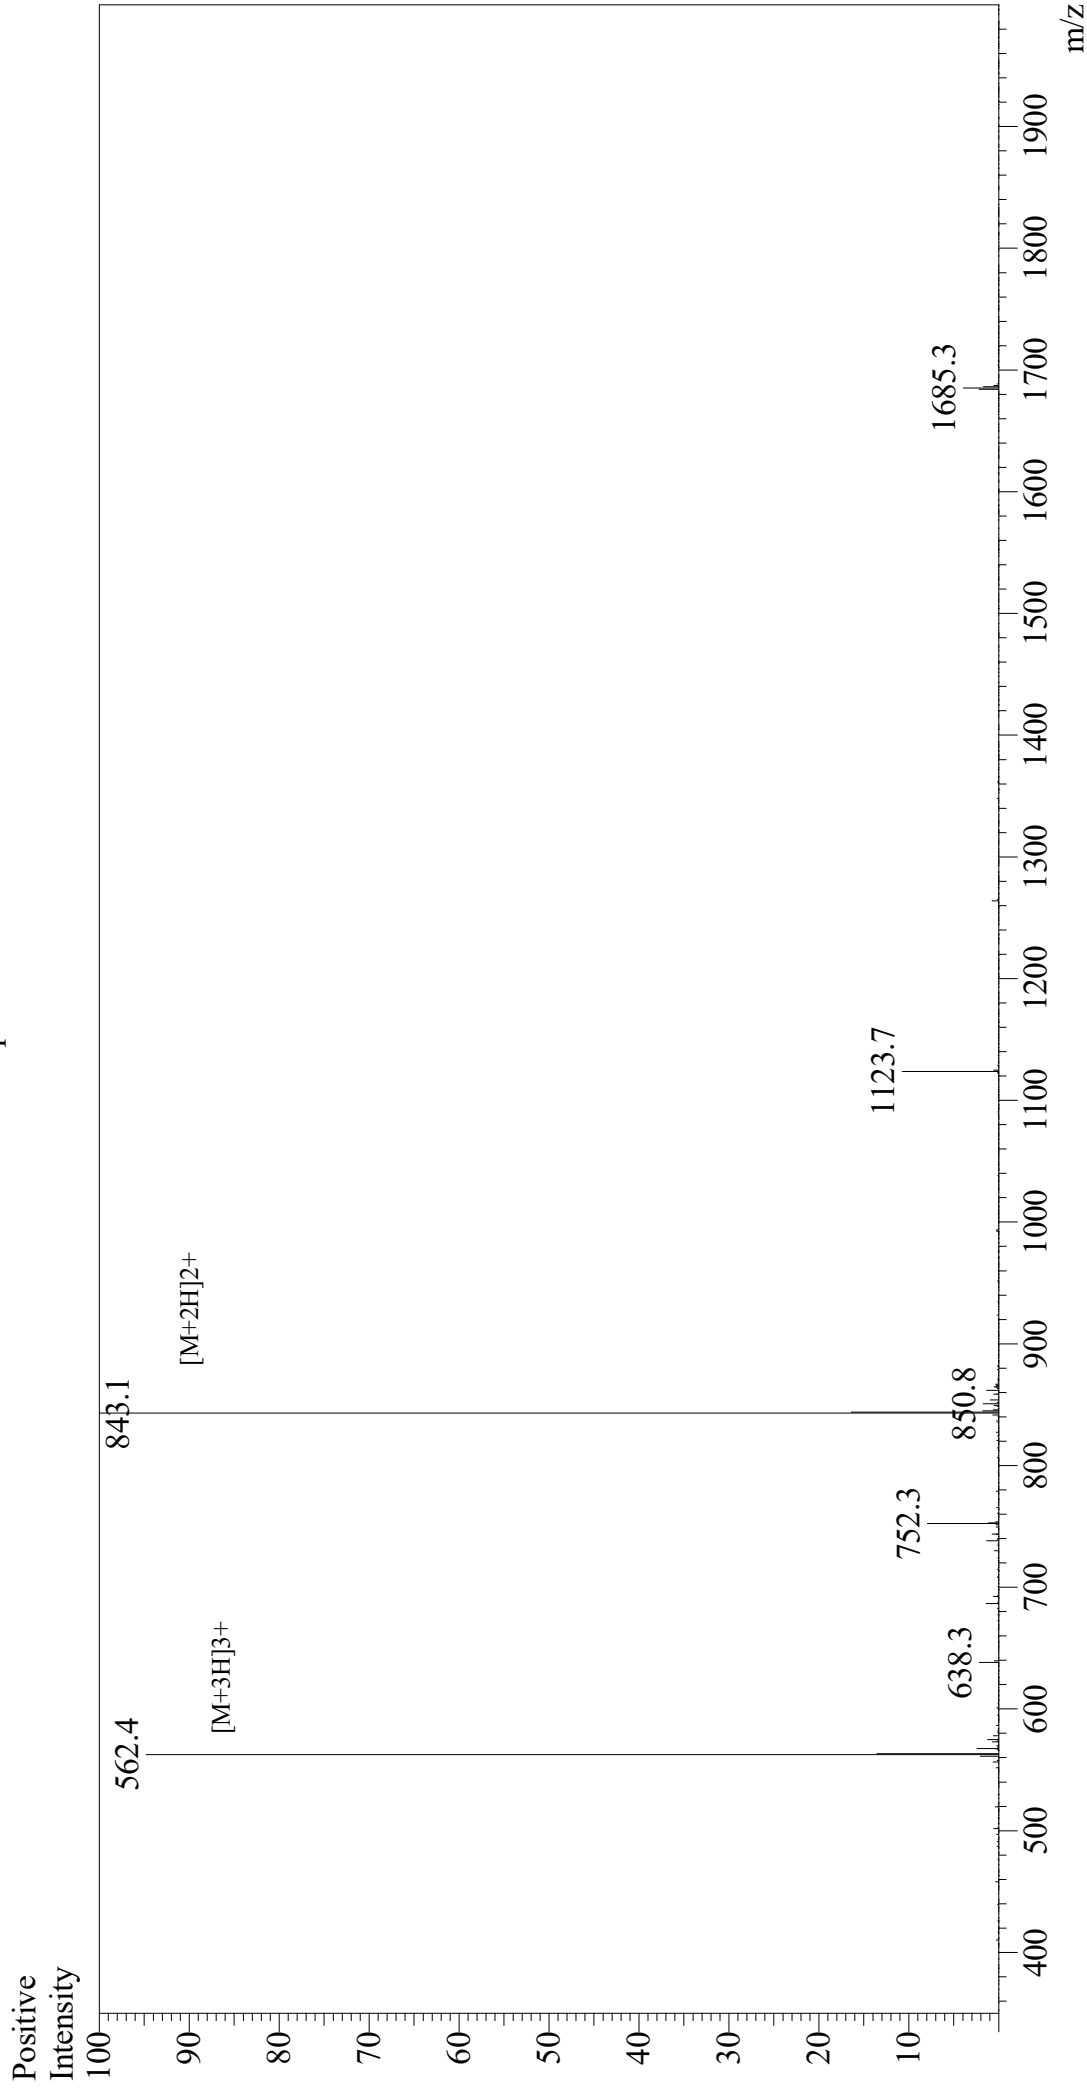

## Sample Information

Month-Day Processed : 05/23/21  
Time Processed : 12:49:35  
Injection Volume : 0.4  
Sample Name :  $\alpha$ -Factor Mating Pheromone, yeast  
Cat No. : RP01002  
Lot No. : E6782721E  
Theoretical MW : 1683.98  
Observed MW : 1684.2

## Interface

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

## Equipment

Equipment : GK11010007  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% H<sub>2</sub>O/50% MeOH