

Sample Name :OVA G4 peptide
 Cat. No. : RP20398
 Lot. No. : E2008521A

Time Processed :6:02:57
 Month-Day-Year Processed :01/10/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010324

<Chromatogram>

mV

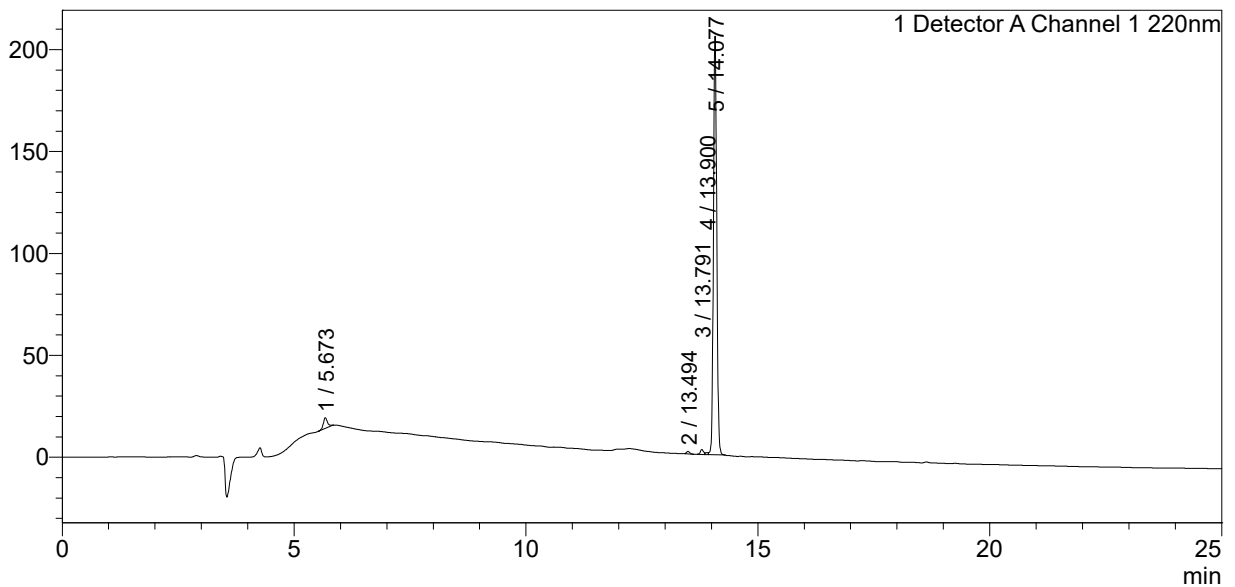

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.673	32135	5168	3.010
2	13.494	5480	1190	0.513
3	13.791	11470	2386	1.074
4	13.900	4126	978	0.386
5	14.077	1014431	205394	95.016
Total		1067643	215117	100.000