

Sample Name :p5 Ligand for Dnak and and DnaJ
 Cat No. :RP20327
 Lot No. :E4915619I
 Time Processed :10:33:49 AM
 Month-Day-Year Processed :09/25/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
30.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

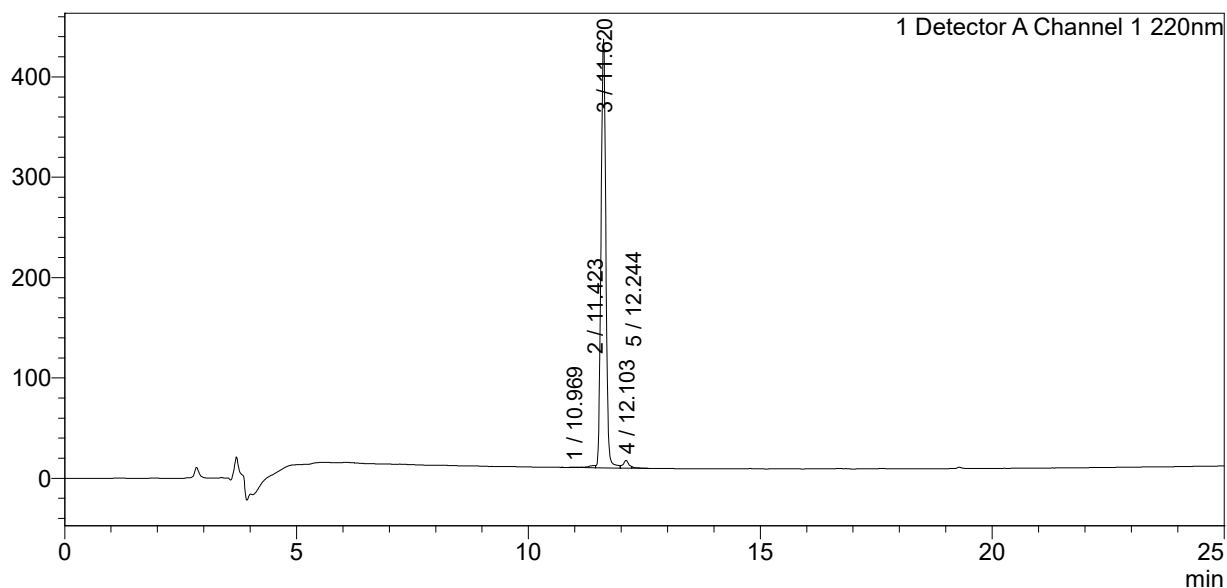

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.969	6097	451	0.190
2	11.423	22527	2189	0.702
3	11.620	3109783	427313	96.890
4	12.103	63643	7714	1.983
5	12.244	7537	1310	0.235
Total		3209587	438977	100.000