

Sample Name : HIV-1 TAT (48-60)  
 Cat. No. : RP20423  
 Lot. No. : PE8991902  
 Time Processed :10:51:38  
 Month-Day-Year Processed :03/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

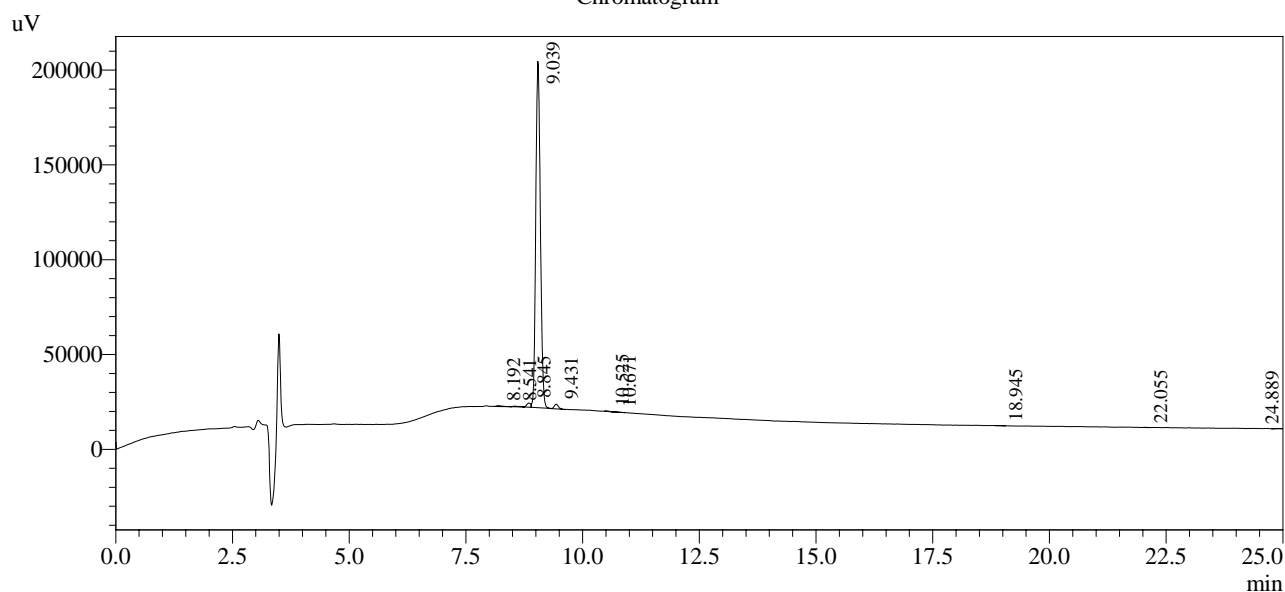

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.192	4220	499	0.326
2	8.541	2789	326	0.216
3	8.845	13287	2203	1.028
4	9.039	1251526	182721	96.821
5	9.431	15196	2492	1.176
6	10.525	1104	207	0.085
7	10.671	1227	98	0.095
8	18.945	1178	158	0.091
9	22.055	1044	119	0.081
10	24.889	1045	132	0.081
Total		1292615	188954	100.000