


Mass Spectrum

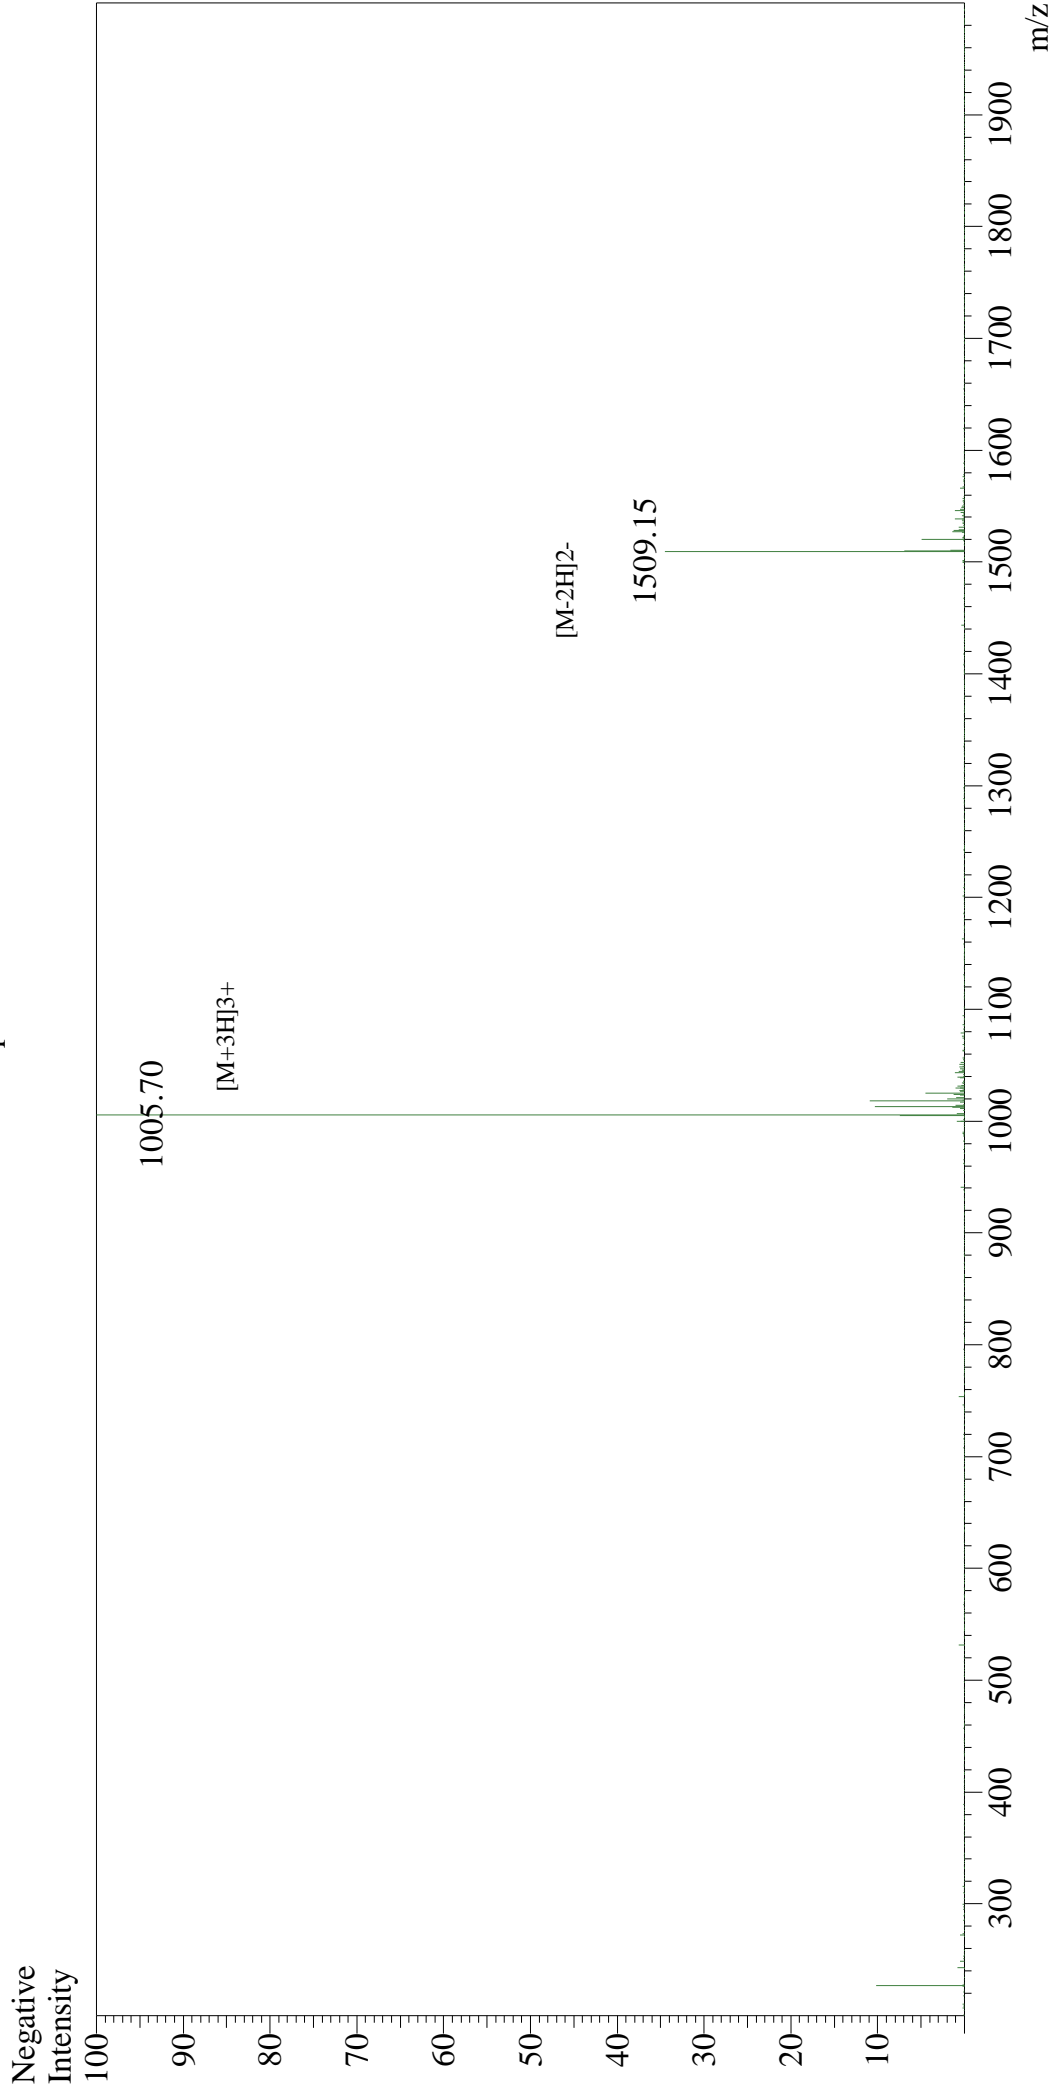

Sample Information

User : Gary
Month-Day Processed : 12/14/17
Time Processed : 17:34:07
Injection Volume : 0.2
Sample Name : C-Peptide (3-33), human
Cat No. : RPI1116
Lot No. : PE4681712
Theoretical MW : 3020.26
Observed MW : 3020.10

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH