

Sample Name :OVA G4 peptide
 Cat No.: RP20398
 Lot No.:E7263020B
 Time Processed :10:35:18
 Month-Day-Year Processed :02/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

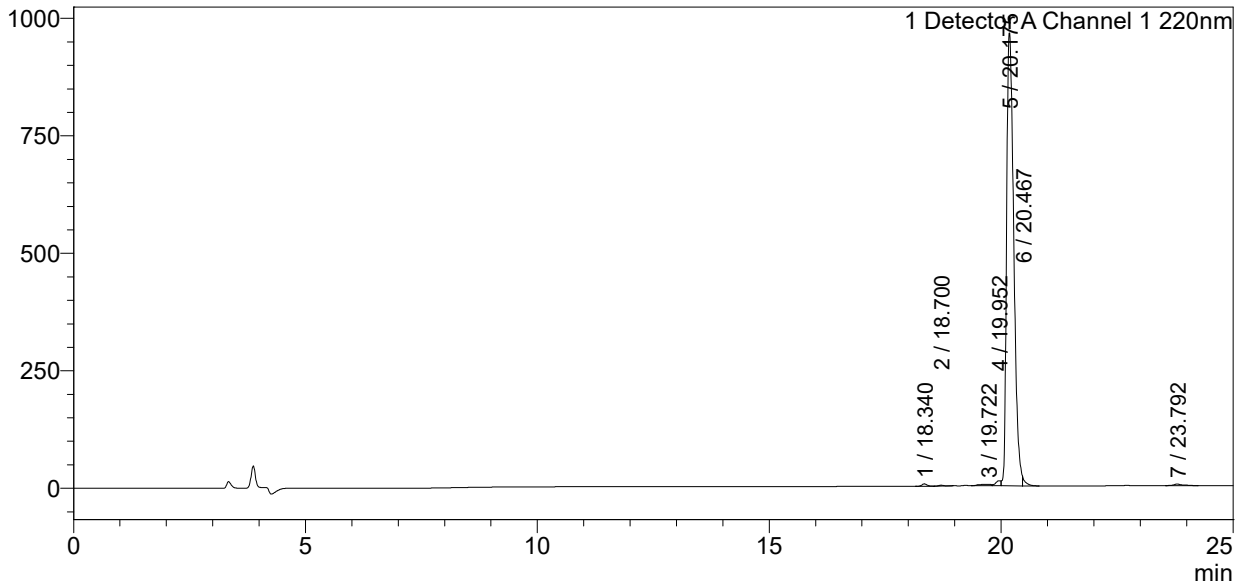

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.340	37270	4975	0.351
2	18.700	10796	1785	0.102
3	19.722	55589	3064	0.524
4	19.952	83752	10681	0.790
5	20.175	10293901	963910	97.078
6	20.467	80641	18338	0.760
7	23.792	41834	3213	0.395
Total		10603783	1005965	100.000