

Sample Name :Melittin  
 Cat No. : RP10290  
 Lot No. : E7538520L  
 Time Processed :3:11:29  
 Month-Day-Year Processed :01/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

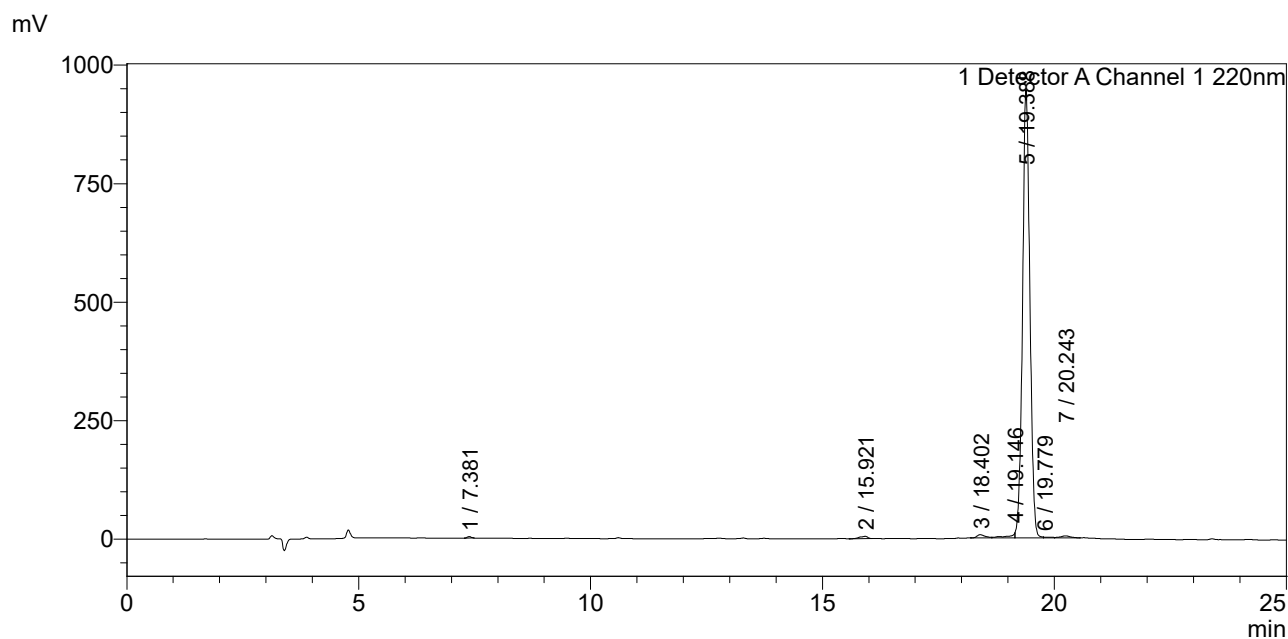

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.381	18095	3212	0.169
2	15.921	56807	4749	0.530
3	18.402	78273	6558	0.730
4	19.146	93084	8959	0.868
5	19.388	10393909	945639	96.970
6	19.779	17692	1549	0.165
7	20.243	60871	4093	0.568
Total		10718731	974759	100.000