

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), human, porcine
 Cat No. :RP11927
 Lot No. :E1325621C
 Time Processed : 20:04:00
 Month-Day-Year Processed : 03/19/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

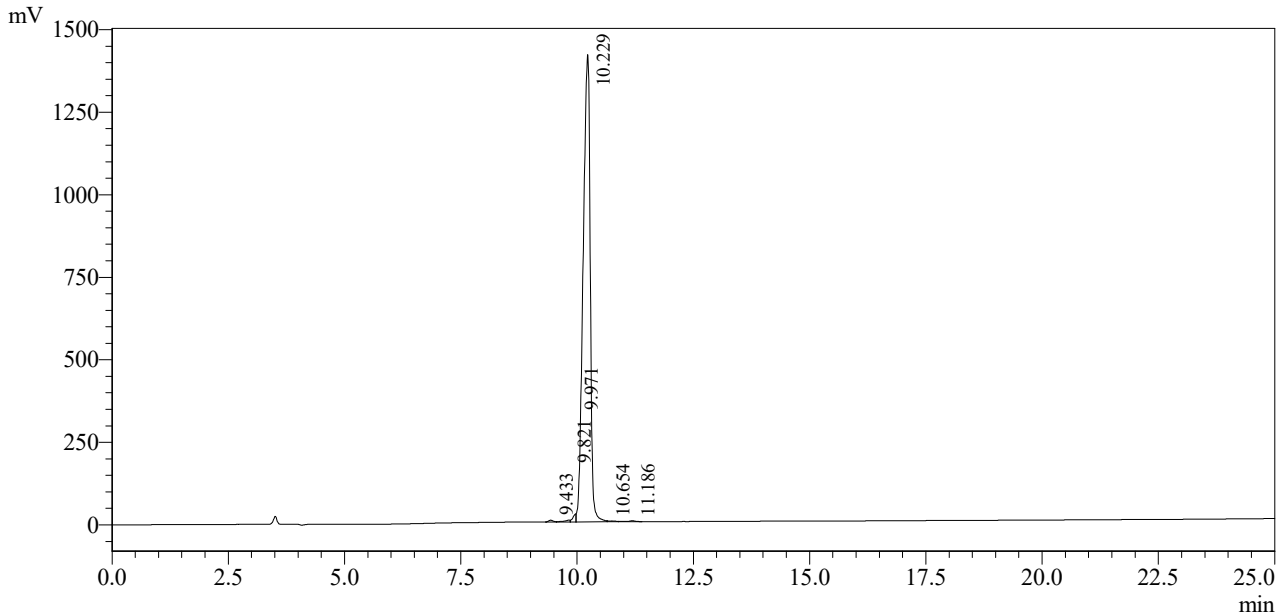

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.433	37811	5535	0.248
2	9.821	46086	5174	0.302
3	9.971	108258	23485	0.710
4	10.229	14999342	1414818	98.357
5	10.654	29464	2577	0.193
6	11.186	28876	2714	0.189
Total		15249836	1454303	100.000