

Sample Name: OVA Peptide (323-339)
 Cat No. : RP10610
 Lot No. : E6214821A
 Time Processed : 13:00:40
 Month-Day-Year Processed : 02/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 25.00 | Pumps | Pump B Conc. | 65 |
| 25.01 | Pumps | Pump B Conc. | 95 |
| 27.00 | Pumps | Pump B Conc. | 95 |
| 27.01 | Pumps | Pump B Conc. | 5 |
| 32.00 | Pumps | Pump B Conc. | 5 |
| 32.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

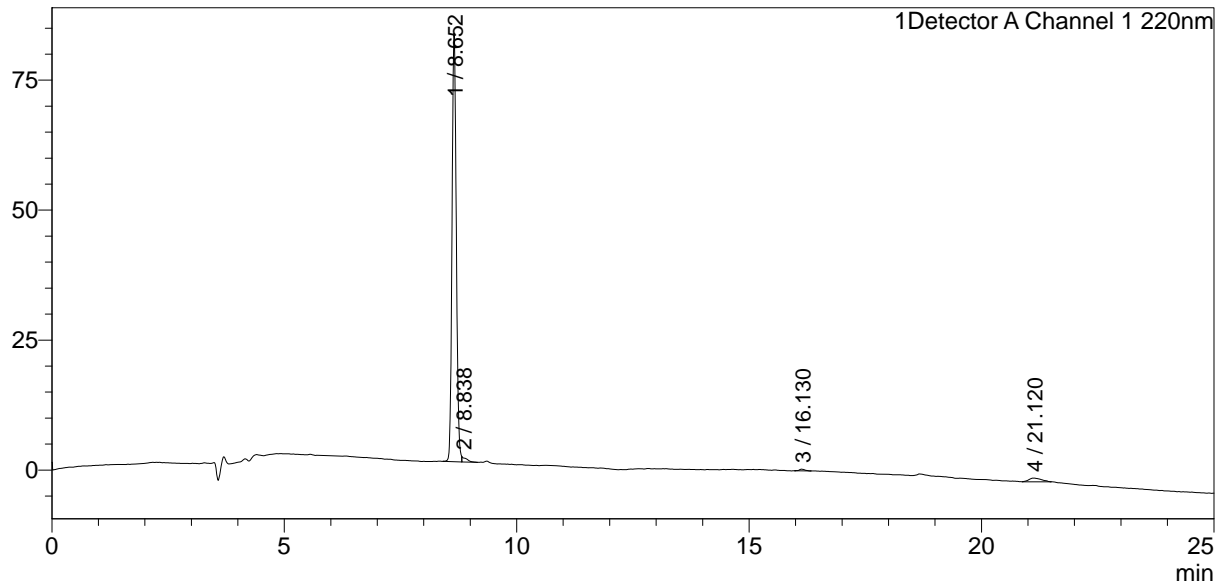

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|--------|--------|---------|
| 1 | 8.652 | 526880 | 81055 | 95.892 |
| 2 | 8.838 | 6819 | 897 | 1.241 |
| 3 | 16.130 | 2624 | 314 | 0.478 |
| 4 | 21.120 | 13127 | 705 | 2.389 |
| Total | | 549451 | 82972 | 100.000 |