

Sample Name: IKK γ NBD Inhibitory Peptide
 Cat No. : RP20478
 Lot No. : E0995221C
 Time Processed : 1:37:02 PM
 Month-Day-Year Processed : 03/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010141

<Chromatogram>

mV

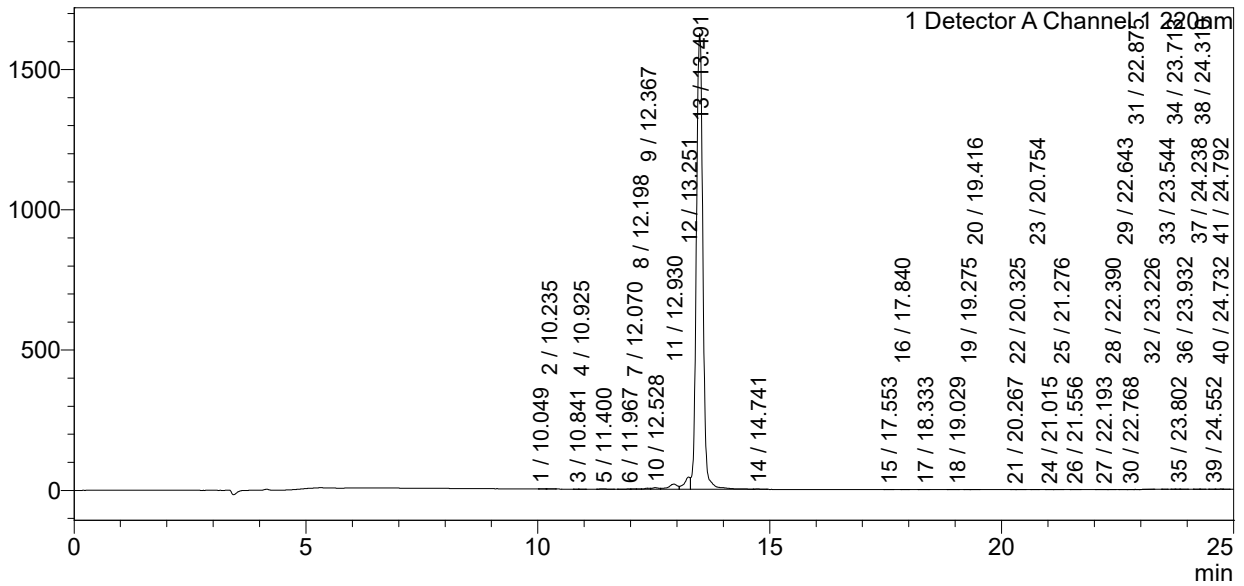

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.049	1131	175	0.007
2	10.235	1464	163	0.009
3	10.841	1050	259	0.006
4	10.925	1049	220	0.006
5	11.400	9523	1394	0.058
6	11.967	4738	499	0.029
7	12.070	4660	668	0.028
8	12.198	4155	686	0.025
9	12.367	30237	3902	0.183
10	12.528	54213	5465	0.328
11	12.930	240382	18354	1.456
12	13.251	386820	43129	2.343
13	13.491	15717505	1624360	95.182
14	14.741	8716	1329	0.053

Peak#	Ret. Time	Area	Height	Area%
15	17.553	1083	135	0.007
16	17.840	1049	176	0.006
17	18.333	1723	210	0.010
18	19.029	2065	315	0.013
19	19.275	1171	206	0.007
20	19.416	1617	208	0.010
21	20.267	1103	249	0.007
22	20.325	1584	216	0.010
23	20.754	1543	243	0.009
24	21.015	1670	233	0.010
25	21.276	2291	310	0.014
26	21.556	2721	308	0.016
27	22.193	3454	333	0.021
28	22.390	2507	322	0.015
29	22.643	2486	275	0.015
30	22.768	1353	224	0.008
31	22.875	1015	219	0.006
32	23.226	2781	242	0.017
33	23.544	1347	233	0.008
34	23.713	1225	295	0.007
35	23.802	1186	231	0.007
36	23.932	1747	260	0.011
37	24.238	1451	282	0.009
38	24.310	1940	355	0.012
39	24.552	1335	213	0.008
40	24.732	2416	338	0.015
41	24.792	1516	239	0.009
Total		16513022	1707473	100.000