

Sample Name : Bid BH3 Peptide  
 Cat.No : RP20440  
 Lot.No : E6096420G  
 Time Processed: 1:50:54  
 Year-Month-Day: 2020/7/13

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

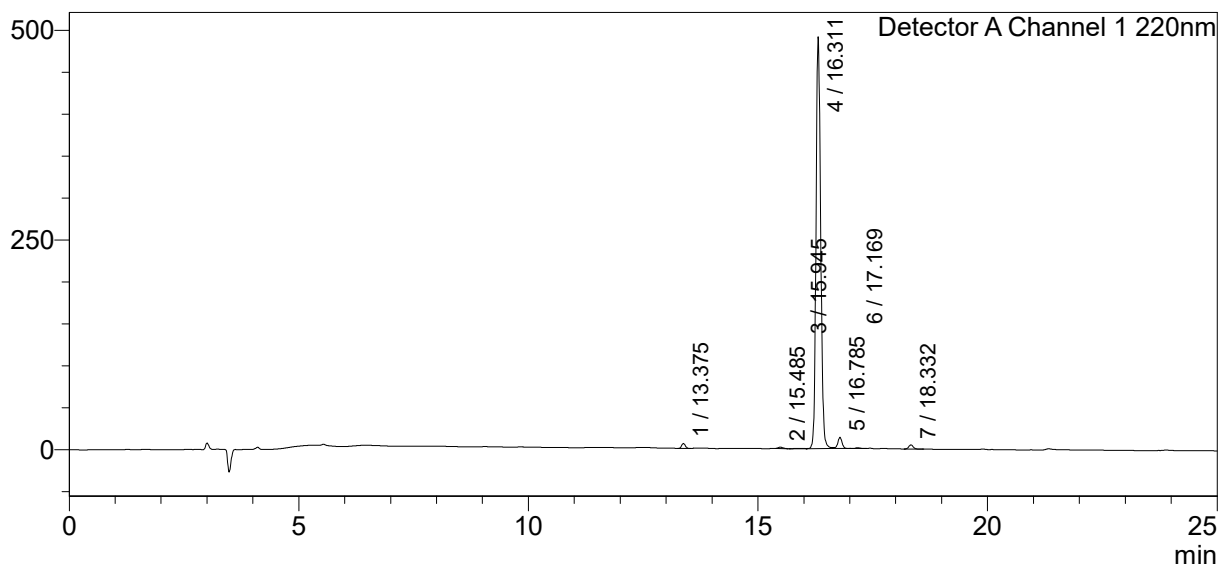

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.375	32435	5981	0.891
2	15.485	11272	1691	0.310
3	15.945	3770	415	0.104
4	16.311	3458874	490761	95.068
5	16.785	90745	13486	2.494
6	17.169	7017	877	0.193
7	18.332	34203	5049	0.940
Total		3638314	518261	100.000