

Sample Name :GLP-1 (7-36), amide, human  
 Cat. No. : RP10773  
 Lot. No. : PE4731810  
 Time Processed : 9:15:46  
 Month-Day-Year Processed : 10/30/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

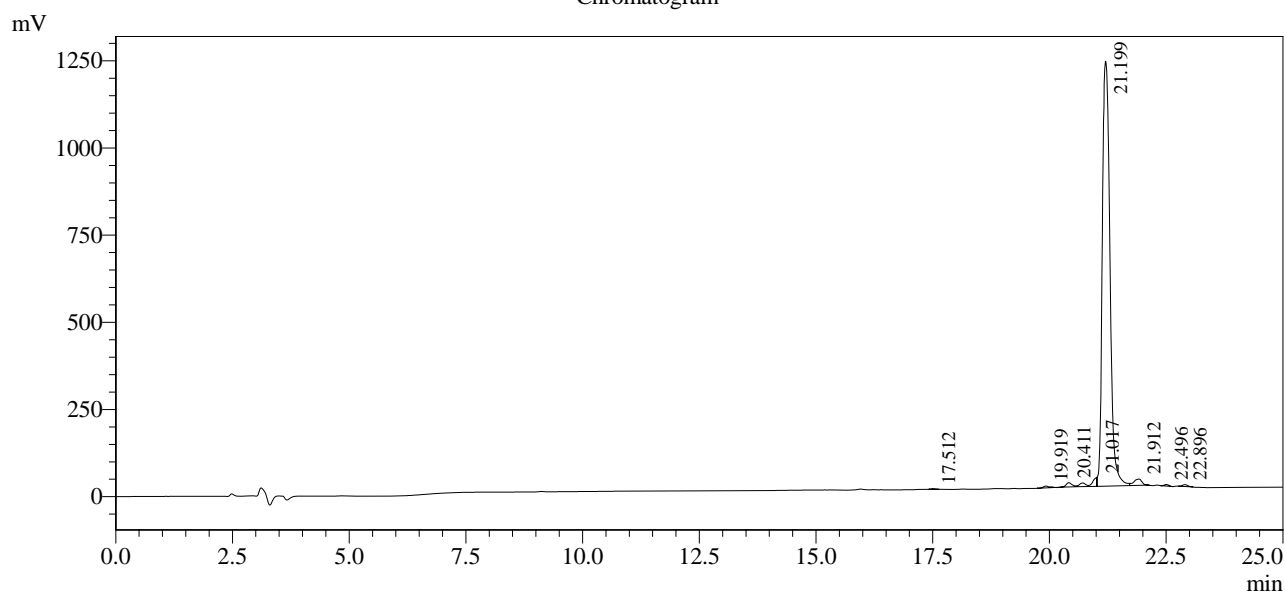

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.512	8738	1518	0.060
2	19.919	45528	5331	0.313
3	20.411	113627	12485	0.781
4	21.017	250919	25471	1.725
5	21.199	13836577	1218585	95.122
6	21.912	222066	18043	1.527
7	22.496	28807	4406	0.198
8	22.896	39895	5344	0.274
Total		14546159	1291183	100.000